

STEMdiff™ Definitive Endoderm Kit



Defined animal component-free medium for the differentiation of human ES and iPS cells to definitive endoderm

Scientists Helping Scientists™ | WWW.STEMCELL.COM

Catalog #05110 1 Kit
#05115 1 Kit

TOLL FREE PHONE 1 800 667 0322 • PHONE +1 604 877 0713

INFO@STEMCELL.COM • TECHSUPPORT@STEMCELL.COM

FOR GLOBAL CONTACT DETAILS VISIT OUR WEBSITE

Product Description

STEMdiff™ Definitive Endoderm Kit is a complete, serum- and animal component-free medium and supplement kit that supports highly efficient differentiation of human embryonic stem (ES) cells and induced pluripotent stem (iPS) cells to definitive endoderm cells. Cells differentiated using STEMdiff™ Definitive Endoderm Kit express high levels of endoderm markers, including CD184 (CXCR4), SOX17, FOXA2, and c-KIT, and lack expression of ectoderm, mesoderm, and pluripotency markers. The definitive endoderm cells produced using this kit are multipotent and capable of further differentiation towards cells of the pancreatic, intestinal, pulmonary, and hepatic lineages, thus providing a robust tool for developmental studies, disease modeling, and drug discovery.

STEMdiff™ Definitive Endoderm Kit (Catalog #05110) and STEMdiff™ Definitive Endoderm Kit (TeSR™-E8™ Optimized; Catalog #05115) have been optimized for the differentiation of human ES and iPS cells cultured in mTeSR™1 (Catalog #85850) or TeSR™-E8™ (Catalog #05990), respectively.

Ordering Information

PRODUCT NAME	CATALOG #	SIZE	COMPONENTS
STEMdiff™ Definitive Endoderm Kit	05110	1 Kit	<ul style="list-style-type: none">• STEMdiff™ Endoderm Basal Medium (100 mL)• STEMdiff™ Definitive Endoderm Supplement MR (100X; 0.35 mL)• STEMdiff™ Definitive Endoderm Supplement CJ (100X; 1.1 mL)
STEMdiff™ Definitive Endoderm Kit (TeSR™-E8™ Optimized)	05115	1 Kit	<ul style="list-style-type: none">• STEMdiff™ Endoderm Basal Medium (100 mL)• STEMdiff™ Definitive Endoderm Supplement MR (100X; 0.35 mL)• STEMdiff™ Definitive Endoderm Supplement CJ (100X; 1.1 mL)• STEMdiff™ Definitive Endoderm TeSR™-E8™ Supplement (20X; 7 mL)

Component Storage and Stability

The following components are sold as part of the STEMdiff™ Definitive Endoderm Kits (see Ordering Information) and are not available for individual sale.

COMPONENT NAME	COMPONENT #	STORAGE	SHELF LIFE
STEMdiff™ Endoderm Basal Medium	05111	Store at -20°C.	Stable until expiry date (EXP) on label.
STEMdiff™ Definitive Endoderm Supplement MR (100X)	05112	Store at -20°C.	Stable until expiry date (EXP) on label.
STEMdiff™ Definitive Endoderm Supplement CJ (100X)	05113	Store at -20°C.	Stable until expiry date (EXP) on label.
STEMdiff™ Definitive Endoderm TeSR™-E8™ Supplement (20X)	05116	Store at 2 - 8°C.	Stable for 12 months from date of manufacture (MFG) on label.

Handling Frozen Components

05111 STEMdiff™ Endoderm Basal Medium

- Thaw entire bottle at room temperature (15 - 25°C) or overnight at 2 - 8°C, and mix thoroughly. Once thawed, use immediately or store at 2 - 8°C for up to 2 months. Alternatively, aliquot and store at -20°C until the expiry date as indicated on the label. After thawing the aliquots, use immediately or store at 2 - 8°C for up to 2 weeks. Do not re-freeze.

05112 STEMdiff™ Definitive Endoderm Supplement MR (100X) OR 05113 STEMdiff™ Definitive Endoderm Supplement CJ (100X)


- Thaw on ice and keep on ice until use. Once thawed, mix thoroughly and use immediately or aliquot and store at -20°C. Do not exceed the expiry date as indicated on the label. After thawing the aliquots, use immediately. Do not re-freeze.

Materials Required But Not Included

PRODUCT NAME	CATALOG #
mTeSR™1 OR TeSR™-E8™	85850 OR 05990
Corning® Matrigel® hESC-qualified matrix OR Vitronectin XF™*	Corning 354277 OR 07180*
Costar® 6-Well Flat-Bottom Plate, Tissue Culture-Treated OR Non Tissue Culture-Treated 6-Well Plates	38015 OR 27147
Gentle Cell Dissociation Reagent	07174
DMEM/F-12 with 15 mM HEPES	36254
Y-27632	72302
D-PBS (Without Ca++ and Mg++)	37350

*If using Vitronectin XF™, CellAdhere™ Dilution Buffer (Catalog #07183) is also required. Alternatively, Vitronectin XF™ Kit with GCDR (Catalog #07190) includes CellAdhere™ Dilution Buffer, Gentle Cell Dissociation Reagent, and Non Tissue Culture-Treated 6-Well Plates.

Schematic of STEMdiff™ Definitive Endoderm Kit Procedure

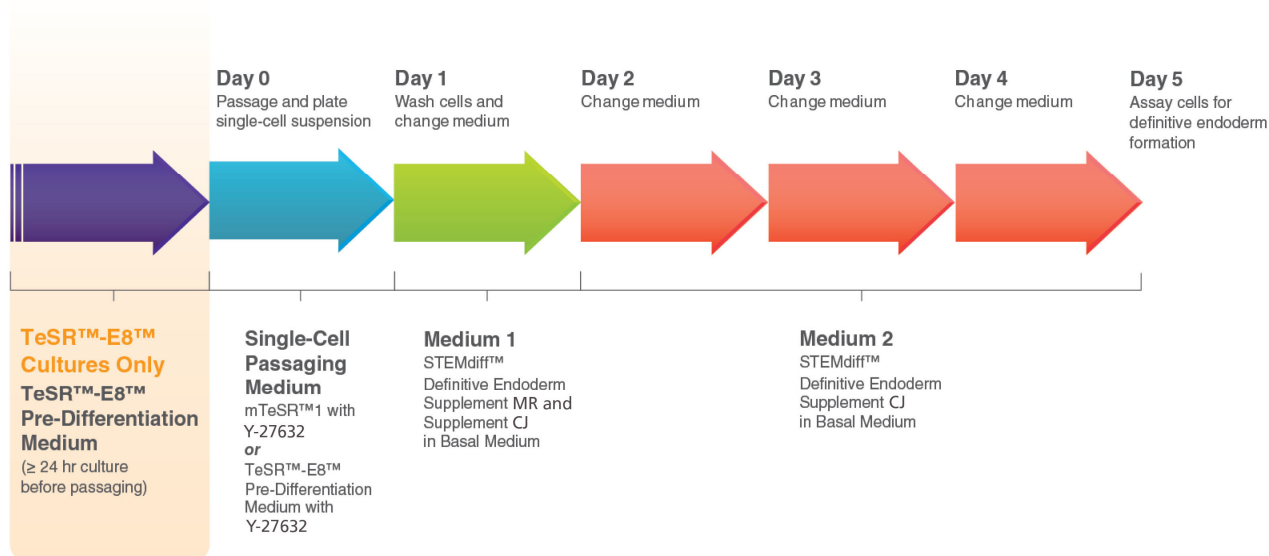

Directions for Use

Please read the entire protocol before proceeding.

NOTE: For complete instructions on coating plates with Corning® Matrigel® or Vitronectin XF™, and maintaining high-quality human ES and iPS cells for use in differentiation, please refer to the Technical Manual: Maintenance of Human Pluripotent Stem Cells in mTeSR™1 (Document #28315) or TeSR™-E8™ (Document #29267), available at www.stemcell.com or contact us to request a copy. Matrix-coated plates should be prepared in advance and be brought to room temperature (15 - 25°C) for at least 30 minutes prior to use.

Use sterile techniques when performing the following protocols. The following are instructions for use with 6-well plates. Indicated volumes are for a single well. If using alternative cultureware, adjust volumes accordingly.

A. PASSAGING CELLS FOR DEFINITIVE ENDODERM INDUCTION

For optimal product performance, passage human ES or iPS cells using the specific passaging protocols for cells cultured in mTeSR™1 or TeSR™-E8™ as outlined in this section, before proceeding with differentiation to definitive endoderm (section B).

NOTE: Human ES and iPS cells are ready for passage when cultures are approximately 70% confluent.

mTeSR™1 Cultures

This protocol is specific to human ES and iPS cells cultured in mTeSR™1 medium.

Day 0

1. Coat plate(s) with Corning® Matrigel® or Vitronectin XF™.
NOTE: If using Corning® Matrigel®, use tissue culture-treated plates; if using Vitronectin XF™, use non-tissue culture-treated plates.
2. Warm (15 - 25°C) sufficient volumes of mTeSR™1, DMEM/F-12, and Gentle Cell Dissociation Reagent for passaging.
3. Prepare Single-Cell Passaging Medium by adding Y-27632 to mTeSR™1 to a final concentration of 10 µM.
4. Wash the well to be passaged with 1 mL of D-PBS (Without Ca⁺⁺ and Mg⁺⁺).
5. Aspirate wash medium and add 1 mL of Gentle Cell Dissociation Reagent.
6. Incubate at 37°C for 8 - 10 minutes.
7. Dislodge cells by pipetting up and down 1 - 3 times using a pipettor with a 1 mL tip. Ensure all remaining cell aggregates are broken up into single cells.
8. Immediately transfer cells to a tube containing an equal volume of DMEM/F-12. Wash the well once with 1 mL of DMEM/F-12 to collect any remaining cells and transfer to the tube. Centrifuge the tube at 300 x *g* for 5 minutes.
9. Resuspend cells in 1 mL of Single-Cell Passaging Medium and count the number of live cells using a hemocytometer.
10. Add cells at a density of 2.1 x 10⁵ cells/cm² (i.e. 2 x 10⁶ cells/well) to coated plates (prepared in step 1). Adjust density if necessary, so that the cells are approximately 90 - 100% confluent on Day 1.
11. Incubate at 37°C for 24 hours.
12. Continue to section B for differentiation.

TeSR™-E8™ Cultures

This protocol is specific to human ES and iPS cells cultured in TeSR™-E8™ medium.

1. Follow a standard passaging protocol to passage TeSR™-E8™ cultures into one well of a 6-well plate, and perform daily medium changes for 4 days.
NOTE: Refer to the Technical Manual: Maintenance of Human Pluripotent Stem Cells in TeSR™-E8™ (Document #29267) for recommended passaging protocols using TeSR™-E8™.
2. Four days after passaging TeSR™-E8™ cultures, prepare complete TeSR™-E8™ Pre-Differentiation Medium as follows:
Add cold (2 - 8°C) STEMdiff™ Definitive Endoderm TeSR™-E8™ Supplement to cold (2 - 8°C) TeSR™-E8™ medium at a 1 in 20 dilution (e.g. add 1 mL of Supplement to 19 mL of TeSR™-E8™). Prepare sufficient complete TeSR™-E8™ Pre-Differentiation Medium to be used until step 6 (i.e. at least 4 mL per well).
NOTE: Complete TeSR™-E8™ Pre-Differentiation Medium can be stored at 2 - 8°C for up to 2 weeks.
3. Warm (15 - 25°C) only the volume of complete TeSR™-E8™ Pre-Differentiation Medium required on this day (i.e. 2 mL per well). Store remaining medium at 2 - 8°C.
4. Aspirate medium from the culture well and add 2 mL of complete TeSR™-E8™ Pre-Differentiation Medium.
5. Incubate at 37°C and perform daily medium changes (steps 3 and 4) until cultures are approximately 70% confluent, and are ready to be passaged.
NOTE: For optimal differentiation performance, cells must be exposed to complete TeSR™-E8™ Pre-Differentiation Medium for at least 24 hours before the next passaging step.

Day 0

6. Passage cells as follows:
 - i. Coat plate(s) with Corning® Matrigel® or Vitronectin XF™.
 - ii. Warm (15 - 25°C) sufficient volumes of complete TeSR™-E8™ Pre-Differentiation Medium, DMEM/F-12, and Gentle Cell Dissociation Reagent for passaging.
 - iii. Prepare Single-Cell Passaging Medium by adding Y-27632 to TeSR™-E8™ Pre-Differentiation Medium to a final concentration of 10 µM.
 - iv. Wash the well to be passaged with 1 mL of D-PBS (Without Ca⁺⁺ and Mg⁺⁺).
 - v. Aspirate wash medium and add 1 mL of Gentle Cell Dissociation Reagent.
 - vi. Incubate at 37°C for 8 - 10 minutes.
 - vii. Dislodge cells by pipetting up and down 1 - 3 times using a pipettor with a 1 mL tip. Ensure all remaining cell aggregates are broken up into single cells.

- viii. Immediately transfer cells to a tube containing an equal volume of DMEM/F-12. Wash the well once with 1 mL of DMEM/F-12 to collect any remaining cells and transfer to the tube. Centrifuge the tube at 300 x g for 5 minutes.
- ix. Resuspend cells in 1 mL of Single-Cell Passaging Medium and count the number of live cells using a hemocytometer.
- x. Plate cells at a density of 2.1×10^5 cells/cm² (i.e. 2×10^6 cells/well) onto coated plates (prepared in step i). Adjust density if necessary, so that the cells are approximately 90 - 100% confluent on Day 1.
- xi. Incubate at 37°C for 24 hours.
- xii. Continue to section B for differentiation.

B. DIFFERENTIATING MONOLAYER CULTURES TO DEFINITIVE ENDODERM

1. **Day 1.** Warm (37°C) sufficient volumes of DMEM/F-12 and STEMdiff™ Endoderm Basal Medium for Day 1 use.
2. Prepare Medium 1 as follows:
 - i. Thaw STEMdiff™ Definitive Endoderm Supplement MR and STEMdiff™ Definitive Endoderm Supplement CJ on ice.
 - ii. Dilute both supplements 1 in 100 in STEMdiff™ Endoderm Basal Medium (e.g. add 10 µL of Supplement MR and 10 µL of Supplement CJ to 980 µL of Basal Medium).
3. Aspirate medium from the well and wash with 1 mL of DMEM/F-12.
4. Aspirate wash medium and replace with 2 mL of Medium 1.
5. Incubate at 37°C for 24 hours.
6. **Day 2.** Prepare Medium 2 as follows:
 - i. Thaw STEMdiff™ Definitive Endoderm Supplement CJ on ice.
 - ii. Add Supplement CJ to cold (2 - 8°C) STEMdiff™ Endoderm Basal Medium at a 1 in 100 dilution (e.g. add 10 µL of Supplement CJ to 990 µL of Basal Medium).
NOTE: Prepare sufficient Medium 2 to be used on Days 2, 3, and 4 (i.e. 6 mL per well).
7. Warm (37°C) only the volume of Medium 2 required for Day 2 use (i.e. 2 mL per well). Store remaining Medium 2 at 2 - 8°C.
8. Aspirate medium from the well and add 2 mL of Medium 2.
NOTE: A wash step with DMEM/F-12 is not required at this step or during subsequent medium changes.
9. Incubate at 37°C for 24 hours.
10. **Day 3.** Warm (37°C) only the volume of Medium 2 required for Day 3 use (i.e. 2 mL per well). Store remaining Medium 2 at 2 - 8°C.
11. Aspirate medium from the well and add 2 mL of Medium 2.
12. Incubate at 37°C for 24 hours.
13. **Day 4.** Warm (37°C) only the volume of Medium 2 required for the Day 4 medium change (i.e. 2 mL per well).
14. Aspirate medium from the well and add 2 mL of Medium 2.
15. Incubate at 37°C for 24 hours.
16. **Day 5.** Cells are ready to be assayed for the formation of definitive endoderm or carried forward into more specialized lineage differentiation protocols.
NOTE: Expression of definitive endoderm markers may peak by Day 4 in some cell lines.

Assessment of Definitive Endoderm Cells

Purity of definitive endoderm cells can be measured by flow cytometry after labeling with fluorochrome-conjugated anti-CXCR4 (e.g. Anti-Human CD184 [CXCR4] Antibody, Clone 12G5, Catalog #60089) and anti-c-Kit (e.g. Anti-Human CD117 [c-Kit] Antibody, Clone 104D2, Catalog #60087) or anti-SOX17 antibodies. Results may vary depending on cell line used.

Related Products

For related products, including specialized media, matrices, antibodies, cytokines, and small molecules, visit www.stemcell.com/DEworkflow or contact us at techsupport@stemcell.com.

STEMCELL TECHNOLOGIES INC.'S QUALITY MANAGEMENT SYSTEM IS CERTIFIED TO ISO 13485. PRODUCTS ARE FOR RESEARCH USE ONLY AND NOT INTENDED FOR HUMAN OR ANIMAL DIAGNOSTIC OR THERAPEUTIC USES UNLESS OTHERWISE STATED.

Copyright © 2018 by STEMCELL Technologies Inc. All rights reserved including graphics and images. STEMCELL Technologies & Design, STEMCELL Shield Design, Scientists Helping Scientists, CellAdhere, and STEMdiff are trademarks of STEMCELL Technologies Canada Inc. mTeSR, TeSR and E8 are trademarks of WARF. Corning, Costar, and Matrigel are registered trademarks of Corning Incorporated. Vitronectin XF is developed and manufactured by Primorigen Biosciences Inc., and Vitronectin XF is a trademark of Primorigen Biosciences, Inc. All other trademarks are the property of their respective holders. While STEMCELL has made all reasonable efforts to ensure that the information provided by STEMCELL and its suppliers is correct, it makes no warranties or representations as to the accuracy or completeness of such information.