

Version 9 Last updated 3 December 2018

ab100545 Human IGF1 ELISA Kit

For the quantitative measurement of human IGF1 in serum, plasma and cell culture supernatants.

This product is for research use only and is not intended for diagnostic use.

Table of Contents

1. Overview	3
2. Protocol Summary	4
3. Precautions	5
4. Storage and Stability	5
5. Limitations	6
6. Materials Supplied	6
7. Materials Required, Not Supplied	7
8. Technical Hints	8
9. Reagent Preparation	9
10. Standard Preparation	10
11. Sample Preparation	11
12. Plate Preparation	11
13. Assay Procedure	12
14. Typical Data	14
15. Typical Sample Values	15
16. Assay Specificity	16
17. Species Reactivity	16
18. Troubleshooting	17
19. Notes	18

1. Overview

Abcam's Human IGF1 ELISA (Enzyme-Linked Immunosorbent Assay) kit is an in vitro enzyme linked immunosorbent assay for the quantitative measurement of Human IGF1 in serum, plasma, and cell culture supernatants.

This ELISA kit can only detect the free form of human IGF-1. It does not detect the complex or bound forms such as IGFBP-bound IGF1.

This assay employs an antibody specific for Human IGF1 coated on a 96-well plate. Standards and samples are pipetted into the wells and IGF1 present in a sample is bound to the wells by the immobilized antibody. The wells are washed and biotinylated anti-Human IGF1 antibody is added. After washing away unbound biotinylated antibody, HRP-conjugated streptavidin is pipetted to the wells. The wells are again washed, a TMB substrate solution is added to the wells and color develops in proportion to the amount of IGF1 bound. The Stop Solution changes the color from blue to yellow, and the intensity of the color is measured at 450 nm.

2. Protocol Summary

Prepare all reagents, samples, and standards as instructed.



Add standard or sample to appropriate wells. Incubate at room temperature.



Add prepared biotin antibody to each well. Incubate at room temperature.



Add prepared Streptavidin Solution. Incubate at room temperature.



Add TMB One-Step Development Solution to each well. Incubate at room temperature.



Add Stop Solution to each well. Read at 450 nm immediately.

3. Precautions

Please read these instructions carefully prior to beginning the assay.

- All kit components have been formulated and quality control tested to function successfully as a kit.
- We understand that, occasionally, experimental protocols might need to be modified to meet unique experimental circumstances. However, we cannot guarantee the performance of the product outside the conditions detailed in this protocol booklet.
- Reagents should be treated as possible mutagens and should be handled with care and disposed of properly. Please review the Safety Datasheet (SDS) provided with the product for information on the specific components.
- Observe good laboratory practices. Gloves, lab coat, and protective eyewear should always be worn. Never pipet by mouth. Do not eat, drink or smoke in the laboratory areas.
- All biological materials should be treated as potentially hazardous and handled as such. They should be disposed of in accordance with established safety procedures.

4. Storage and Stability

Store kit at -20°C immediately upon receipt. Kit has a storage time of 1 year from receipt, providing components have not been reconstituted.

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in the Materials Supplied section.

5. Limitations

- Assay kit intended for research use only. Not for use in diagnostic procedures.
- Do not mix or substitute reagents or materials from other kit lots or vendors. Kits are QC tested as a set of components and performance cannot be guaranteed if utilized separately or substituted.

6. Materials Supplied

Item	Quantity	Storage Condition
IGF1 Microplate (12 x 8 wells)	96 wells	-20°C
20X Wash Buffer Concentrate	25 mL	-20°C
Recombinant Human IGF1 Standard	2 Vials	-20°C
Assay Diluent C	2 x 30 mL	-20°C
Biotinylated anti-Human IGF1	2 Vials	-20°C
120X HRP-Streptavidin Concentrate	200 µL	-20°C
TMB One-Step Substrate Reagent	12 mL	-20°C
Stop Solution	8 mL	-20°C

7. Materials Required, Not Supplied

These materials are not included in the kit, but will be required to successfully perform this assay:

- Microplate reader capable of measuring absorbance at 450 nm.
- Precision pipettes to deliver 2 μ L to 1 mL volumes.
- Adjustable 1-25 mL pipettes for reagent preparation.
- 100 mL and 1 liter graduated cylinders.
- Absorbent paper.
- Distilled or deionized water.
- Log-log graph paper or computer and software for ELISA data analysis.
- Tubes to prepare standard or sample dilutions.

8. Technical Hints

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers.
- Avoid foaming or bubbles when mixing or reconstituting components.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Ensure plates are properly sealed or covered during incubation steps.
- Complete removal of all solutions and buffers during wash steps.
- When preparing your standards, it is very critical to briefly spin down the vial first. The powder may drop off from the cap when opening it if you do not spin down. Be sure to dissolve the powder thoroughly when reconstituting. After adding Assay Diluent to the vial, we recommend inverting the tube a few times, then flick the tube a few times, and then spin it down; repeat this procedure 3-4 times. This is a technique we find very effective for thoroughly mixing the standard without too much mechanical force.
- Do not vortex the standard during reconstitution, as this will destabilize the protein.
- Once your standard has been reconstituted, it should be used right away or else frozen for later use.
- Keep the standard dilutions on ice while during preparation, but the ELISA procedure should be done at room temperature.
- Be sure to discard the working standard dilutions after use – they do not store well.
- This kit is sold based on number of tests. A 'test' simply refers to a single assay well. The number of wells that contain sample, control or standard will vary by product. Review the protocol completely to confirm this kit meets your requirements. Please contact our Technical Support staff with any questions.
- Selected components in this kit are supplied in surplus amount to account for additional dilutions, evaporation, or instrumentation settings where higher volumes are required. They should be disposed of in accordance with established safety procedures.

9. Reagent Preparation

- Equilibrate all reagents to room temperature (18-25°C) prior to use. The kit contains enough reagents for 96 wells.
- Prepare only as much reagent as is needed on the day of the experiment.

9.1 1X Wash Solution

If the 20X Wash Concentrate contains visible crystals, equilibrate to room temperature and mix gently until dissolved. Dilute 20 mL of 20X Wash Buffer Concentrate into deionized or distilled water to yield 400 mL of 1X Wash Buffer.

9.2 1X Biotinylated IGF1 Detection Antibody

Briefly spin the Biotinylated anti-Human IGF1 vial before use. Add 100 µL of 1X Assay Diluent C into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can either be stored at 4°C for 5 days or aliquoted and frozen at -20°C for 2 months). The detection antibody concentrate must be diluted 80-fold with 1X Assay Diluent prior to use in the Assay Procedure.

9.3 1X HRP-Streptavidin Solution

Briefly spin the 120X HRP-Streptavidin concentrate vial and pipette up and down to mix gently before use. HRP-Streptavidin concentrate must be diluted 120-fold with 1X Assay Diluent C prior to use in the Assay Procedure.

For example: Briefly spin the vial and pipette up and down to mix gently. Add 100 µL of 120X HRP-Streptavidin concentrate into a tube with 12 mL 1X Assay Diluent to prepare a 120-fold diluted 1X HRP-Streptavidin solution (don't store the diluted solution for next day use). Mix well.

10. Standard Preparation

- Prepare serially diluted standards immediately prior to use. Always prepare a fresh set of standards for every use.
- Discard working standard dilutions after use as they do not store well.
- Standard should be stored at -80°C after reconstitution.
- The following section describes the preparation of a standard curve for duplicate measurements (recommended).

10.1 Briefly spin the vial of IGF1 Standard. Prepare the 100 ng/mL IGF1 Stock Standard by adding 400 μL 1X Assay Diluent C into the vial (see table below).

10.2 Dissolve the powder thoroughly by gentle mixing.

10.3 Label tubes #1-8.

10.4 Prepare Standard #1 by adding 150 μL of the 100 ng/mL Stock Standard to 350 μL Assay Diluent into tube #1. Mix thoroughly and gently.

10.5 Pipette 300 μL 1X Assay Diluent C into remaining tubes.

10.6 Prepare Standard #2 by transferring 200 μL from tube #1 to #2, mix thoroughly.

10.7 Prepare Standard #3 by transferring 200 μL from tube #2 to #3, mix thoroughly.

10.8 Using the table below as a guide, prepare further serial dilutions.

10.9 1X Assay Diluent serves as the zero standard (0 ng/mL).

Standard #	Volume to Dilute (μL)	Volume Diluent (μL)	Total Volume (μL)	Starting Conc. (ng/mL)	Final Conc. (ng/mL)
1	150	350	500	100	30
2	200	300	500	30	12
3	200	300	500	12	4.8
4	200	300	500	4.8	1.92
5	200	300	500	1.92	0.768
6	200	300	500	0.768	0.307
7	200	300	500	0.307	0.123
8 (Blank)	-	300	300	-	-

11. Sample Preparation

General Sample Information:

- If your samples need to be diluted, 1X Assay Diluent should be used for dilution of serum, plasma and culture supernatants.
- Suggested dilution for normal serum/plasma: 2 - 20 fold.
- Please note that levels of the target protein may vary between different specimens. Optimal dilution factors for each sample must be determined by the investigator.

12. Plate Preparation


- The 96 well plate strips included with this kit are supplied ready to use. It is not necessary to rinse the plate prior to adding reagents.
- Unused well strips should be returned to the plate packet and stored at 4°C.
- For statistical reasons, we recommend each sample should be assayed with a minimum of two replicates (duplicates).
- Well effects have not been observed with this assay. Contents of each well can be recorded on the template sheet included in the Resources section.

13. Assay Procedure

- Equilibrate all materials and prepared reagents to room temperature prior to use.
 - We recommend that you assay all standards, controls and samples in duplicate.
- 13.1** Add 100 μL of each standard (see Standard Preparation section 10) and sample into appropriate wells. Cover well and incubate for 2.5 hours at room temperature or over night at 4°C with gentle shaking.
 - 13.2** Discard the solution and wash 4 times with 1X Wash Solution. Wash by filling each well with 1X Wash Solution (300 μL) using a multi-channel Pipette or auto washer. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining liquid by aspirating or decanting. Invert the plate and blot it against clean paper towels.
 - 13.3** Add 100 μL of 1X Biotinylated IGF1 Detection Antibody (Reagent Preparation section 9) to each well. Incubate for 1 hour at room temperature with gentle shaking.
 - 13.4** Discard the solution. Repeat the wash as in step 13.2.
 - 13.5** Add 100 μL of 1X HRP-Streptavidin solution (see Reagent Preparation section 9) to each well. Incubate for 45 minutes at room temperature with gentle shaking.
 - 13.6** Discard the solution. Repeat the wash as in step 13.2.
 - 13.7** Add 100 μL of TMB One-Step Substrate Reagent to each well. Incubate for 30 minutes at room temperature in the dark with gentle shaking.
 - 13.8** Add 50 μL of Stop Solution to each well. Read at 450 nm immediately.
 - 13.9** Analyze the data as described below.
 - 13.9.1** Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
 - 13.9.2** To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance (OD) on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
 - 13.9.3** Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

14. Typical Data

Typical standard curve – data provided for demonstration purposes only. A new standard curve must be generated for each assay performed.

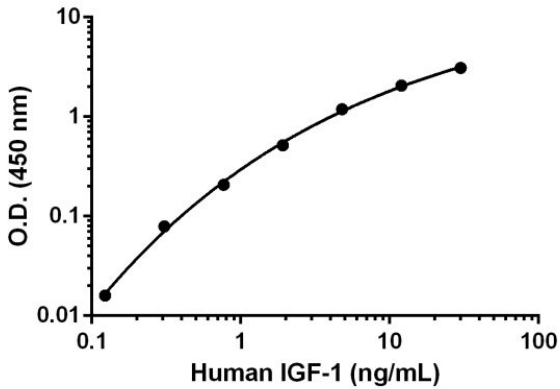

Conc. (ng/mL)	O.D.
	Assay Diluent
0.123	0.016
0.307	0.079
0.768	0.207
1.92	0.517
4.8	1.195
12	2.059
30	3.107

Figure 1. Example of a typical human IGF1 dilution series. Background-subtracted data values (mean +/- SD) are graphed.

15. Typical Sample Values

SENSITIVITY –

The minimum detectable dose of IGF1 is typically less than 0.1 ng/mL.

PRECISION –

	Intra-assay Precision	Inter-Assay Precision
CV (%)	<10%	<12%

RECOVERY –

Recovery was determined by spiking Human IGF1 into normal Human serum, plasma and cell culture media. Mean recoveries are as follows:

Sample Type	Average % Recovery	Range %
Serum	119.6	105-138
Plasma	105.4	81-121
Cell Culture Media	102.5	98-110

Linearity of Dilution

Serum Dilution	Average % Expected Value	Range (%)
1:2	116.4	108-124
1:4	121.9	114-130

Plasma Dilution	Average % Expected Value	Range (%)
1:2	111.9	107-125
1:4	104.6	81-120

Cell Culture Media Dilution	Average % Expected Value	Range (%)
1:2	103.3	94-118
1:4	84.62	77-92

16. Assay Specificity

Cross Reactivity: This ELISA kit shows no cross-reactivity with the following cytokines tested: Human Angiogenin, BDNF, BLC, ENA-78, FGF-4, IGFBP-1, IGFBP-2, IGFBP-3, IGFBP-4, IL-1 α , IL-1 β , IL-2, IL-3, IL-4, IL-5, IL-6, IL-7, IL-8, IL-9, IL-10, IL-11, IL-12 p70, IL-12 p40, IL-13, IL-15, IL-309, IP-10, G-CSF, GM-CSF, IFN- γ , Leptin (OB), MCP-1, MCP-3, MDC, MIP-1 α , MIP-1 β , MIP-1, PARC, RANTES, SCF, TARC, TGF- β , TIMP-1, TIMP-2, TNF- α , TNF- β , TPO, VEGF).

17. Species Reactivity

This kit detects human IGF1 in serum, plasma and cell culture supernatants.

Please contact our Technical Support team for more information.

18. Troubleshooting

Problem	Reason	Solution
Poor standard curve	Inaccurate pipetting	Check pipettes
	Improper standard dilution	Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing
Low signal	Incubation times too brief	Ensure sufficient incubation times; increase to 2 or 3 hours standard/sample incubation
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
Large CV	Inaccurate pipetting	Check pipettes
High background	Plate is insufficiently washed	Review manual for proper wash technique. If using a plate washer, check all ports for obstructions
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	Store the reconstituted proteins at -80°C , all other assay components 4°C . Keep substrate solution protected from light.

19. Notes

Technical Support

Copyright © 2017 Abcam, All Rights Reserved. The Abcam logo is a registered trademark. All information / detail is correct at time of going to print.

Austria

wissenschaftlicherdienst@abcam.com | 019-288-259

France

supportscientifique@abcam.com | 01.46.94.62.96

Germany

wissenschaftlicherdienst@abcam.com | 030-896-779-154

Spain

soportecientifico@abcam.com | 91-114-65-60

Switzerland

technical@abcam.com

Deutsch: 043-501-64-24 | Français: 061-500-05-30

UK, EU and ROW

technical@abcam.com | +44(0)1223-696000

Canada

ca.technical@abcam.com | 877-749-8807

US and Latin America

us.technical@abcam.com | 888-772-2226

Asia Pacific

hk.technical@abcam.com | (852) 2603-6823

China

cn.technical@abcam.com | +86-21-5110-5938 | 400-628-6880

Japan

technical@abcam.co.jp | +81-(0)3-6231-0940

Singapore

sg.technical@abcam.com | 800 188-5244

Australia

au.technical@abcam.com | +61-(0)3-8652-1450

New Zealand

nz.technical@abcam.com | +64-(0)9-909-7829