

Version 4 Last updated 4 September 2019

ab213805 – Human LBP ELISA Kit

For the quantitative detection of Human LBP in cell culture supernatants, cell lysates, serum and plasma (heparin, EDTA).

This product is for research use only and is not intended for diagnostic use.

Table of Contents

1. Overview	1
2. Protocol Summary	2
3. Precautions	3
4. Storage and Stability	3
5. Limitations	4
6. Materials Supplied	4
7. Materials Required, Not Supplied	5
8. Technical Hints	6
9. Reagent Preparation	7
10. Standard Preparation	9
11. Sample Preparation	10
12. Assay Procedure	12
13. Calculations	14
14. Typical data	15
15. Typical sample values	16
16. Troubleshooting	17
17. Notes	18

1. Overview

The Human LBP Enzyme-Linked Immunosorbent Assay (ELISA) kit (ab213805) is designed for the quantitative detection of Human LBP in cell culture supernatants, cell lysates, serum and plasma (heparin, EDTA).

The ELISA kit is based on standard sandwich enzyme-linked immunosorbent assay technology. A monoclonal antibody from mouse specific for LBP has been pre-coated onto 96-well plates. Standards (Expression system for standard: NSO; Immunogen sequence: A26-V481) and test samples are added to the wells, a biotinylated detection polyclonal antibody from goat specific for LBP is added subsequently and then followed by washing with PBS or TBS buffer. Avidin-Biotin-Peroxidase Complex was added and unbound conjugates were washed away with PBS or TBS buffer. HRP substrate TMB was used to visualize HRP enzymatic reaction. TMB was catalyzed by HRP to produce a blue color product that changed into yellow after adding acidic TMB Stop Solution. The density of yellow is proportional to the Human LBP amount of sample captured in plate.

Lipopolysaccharide binding protein is a protein that in humans is encoded by the LBP gene. This gene is mapped to 20q11.23. LBP is a soluble acute-phase protein that binds to bacterial lipopolysaccharide (or LPS) to elicit immune responses by presenting the LPS to important cell surface pattern recognition receptors called CD14 and TLR4. It is present in the cerebrospinal fluid of patients with pneumococcal meningitis. The protein encoded by this gene is involved in the acute phase immunologic response to gram-negative bacterial infections. LBP is made in the liver during the acute phase of infections and is thought to function as a carrier for LPS and to help control LPS-dependent monocyte responses.

2. Protocol Summary

Prepare all reagents, samples, and standards as instructed



Add 100 μ L standard or sample to appropriate wells

Incubate at 37°C for 90 minutes



Discard plate content. Do not wash.

Add 100 μ L biotinylated Antibody in to all wells

Incubate at 37°C for 60 minutes



Wash each well three times with 300 μ L 0.01M PBS (or TBS)



Add 100 μ L ABC working solution

Incubate at 37°C for 30 minutes



Wash each well five times with 300 μ L 0.01M PBS (or TBS)

Add 90 μ L of prepared TMB

Incubate at 37°C in dark for 25-30 minutes



Add 100 μ L TMB Stop Solution and read OD at 450 nm within 30 minutes

3. Precautions

Please read these instructions carefully prior to beginning the ELISA assay.

- All kit components have been formulated and quality control tested to function successfully as a kit.
- We understand that, occasionally, experimental protocols might need to be modified to meet unique experimental circumstances. However, we cannot guarantee the performance of the product outside the conditions detailed in this protocol booklet.
- Reagents should be treated as possible mutagens and should be handled with care and disposed of properly. Please review the Safety Datasheet (SDS) provided with the product for information on the specific components.
- Observe good laboratory practices. Gloves, lab coat, and protective eyewear should always be worn. Never pipette by mouth. Do not eat, drink or smoke in the laboratory areas.
- All biological materials should be treated as potentially hazardous and handled as such. They should be disposed of in accordance with established safety procedures.

4. Storage and Stability

Store ELISA kit at -20°C immediately upon receipt.

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in the Materials Supplied section.

Aliquot components in working volumes before storing at the recommended temperature.

5. Limitations

- ELISA kit intended for research use only. Not for use in diagnostic procedures.
- Do not mix or substitute reagents or materials from other kit lots or vendors. Kits are QC tested as a set of components and performance cannot be guaranteed if utilized separately or substituted.

6. Materials Supplied

Item	Quantity	Storage Condition (Before prep)	Storage Condition (After prep)
Anti-Human LBP Coated Microplate (12 x 8 wells)	1 x 96 well plate	-20°C	-20°C
Lyophilized Recombinant Human LBP Standard	2 x 50 ng	-20°C	-20°C
Biotinylated anti-Human LBP Antibody	130 µL	-20°C	-20°C
Avidin-Biotin-Peroxidase Complex (ABC)	130 µL	-20°C	-20°C
Sample Diluent Buffer	30 mL	-20°C	-20°C
Antibody Diluent Buffer	12 mL	-20°C	-20°C
ABC Diluent Buffer	12 mL	-20°C	-20°C
TMB Color Developing Agent	10 mL	-20°C	-20°C
TMB Stop Solution	10 mL	-20°C	-20°C
Adhesive Plate Seal	4	-20°C	-20°C

7. Materials Required, Not Supplied

These materials are not included in the kit, but will be required to successfully perform this assay:

- Microplate reader capable of measuring absorbance at 450 nm.
- Automated plate washer.
- Multi- and single-channel pipettes.
- Clean tubes and Eppendorf tubes.
- Washing buffer (neutral 0.01M PBS or 0.01M TBS).

Preparation of 0.01M TBS: Add 1.2 g Tris, 8.5 g NaCl; 450 μ L of purified acetic acid or 700 μ L of concentrated hydrochloric acid to 1,000 mL distilled water and adjust pH to 7.2~7.6. Finally, adjust the total volume to 1L.

Preparation of 0.01 M PBS: Add 8.5 g sodium chloride, 1.4 g Na_2HPO_4 and 0.2 g NaH_2PO_4 to 1,000 mL distilled water and adjust pH to 7.2~7.6. Finally, adjust the total volume to 1L.

8. Technical Hints

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers.
- Avoid foaming or bubbles when mixing or reconstituting components.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Ensure plates are properly sealed or covered during incubation steps.
- Don't let the 96-well plate dry, for a dry plate will inactivate active components on plate.
- Complete removal of all solutions and buffers during wash steps is necessary to minimize background.
- All samples should be mixed thoroughly and gently.
- Avoid multiple freeze/thaw of samples.
- When generating positive control samples, it is advisable to change pipette tips after each step.
- Before using the kit, spin tubes and bring down all components to the bottom of tubes.
- In order to avoid marginal effect of plate incubation due to temperature difference (reaction may be stronger in the marginal wells), it is suggested that the diluted ABC and TMB solution will be pre-warmed in 37°C for 30 minutes before using.
- **To avoid high background always add samples or standards to the well before the addition of the antibody cocktail.**
- **This kit is sold based on number of tests. A 'test' simply refers to a single assay well. The number of wells that contain sample, control or standard will vary by product. Review the protocol completely to confirm this kit meets your requirements. Please contact our Technical Support staff with any questions.**

9. Reagent Preparation

- Equilibrate all reagents to room temperature (18-25°C) prior to use. The kit contains enough reagents for 96 wells.
- Prepare only as much reagent as is needed on the day of the experiment.

9.1 Anti-Human LBP coated Microplate (12 x 8 wells)

One plate of 96 wells. Ready to use. Store at -20°C.

9.2 Lyophilized recombinant Human LBP standard (2 x 100 ng)

- 9.2.1 LBP standard solution should be prepared no more than 2 hours prior to the experiment. Two tubes of LBP standard (2 x 100 ng) are included in each kit. Use one tube for each experiment.
- 9.2.2 Add 1 mL sample diluent buffer into one tube to create 100 ng/mL of Human LBP stock solution. Keep the tube at room temperature for 10 minutes and mix thoroughly.

9.3 Biotinylated anti-Human LBP antibody

The solution should be prepared no more than 2 hours prior to the experiment.

- 9.3.1 The total volume should be: 100 μ L /well x (the number of wells). (Allowing 100 μ L – 200 μ L more than total volume)
- 9.3.2 Biotinylated anti-Human LBP antibody should be diluted in 1:100 with the antibody diluent buffer and mixed thoroughly. (i.e. Add 1 μ L Biotinylated anti-Human LBP antibody to 99 μ L antibody diluent buffer.)

9.4 Avidin-Biotin-Peroxidase Complex (ABC)

The solution should be prepared no more than 1 hour prior to the experiment.

- 9.4.1 The total volume should be: 100 μ L/well x (the number of wells). (Allowing 100 μ L - 200 μ L more than total volume)
- 9.4.2 Avidin- Biotin-Peroxidase Complex (ABC) should be diluted in 1:100 with the ABC dilution buffer and mixed thoroughly. (i.e. Add 1 μ L ABC to 99 μ L ABC diluent buffer.)

- 9.5 Sample diluent buffer**
30 mL. Ready to use. Store at -20°C.
- 9.6 Antibody diluent buffer**
12 mL. Ready to use. Store at -20°C.
- 9.7 ABC diluent buffer**
12 mL. Ready to use. Store at -20°C.
- 9.8 TMB**
10 mL. Ready to use. Store at -20°C.
- 9.9 TMB Stop Solution**
10 mL. Ready to use. Store at -20°C.

10. Standard Preparation

- 10.1** To prepare standards, label 6 Eppendorf tubes with 50 ng/mL, 25 ng/mL, 12.5 ng/mL, 6.25 ng/mL, 3.125 ng/mL, 1.5625 ng/mL and 0.7813 ng/mL respectively.
- 10.2** Aliquot 300 μ L of the sample diluent buffer into each tube.
- 10.3** Add 300 μ L of the above 100 ng/mL LBP solution into 1st tube and mix.
- 10.4** Transfer 300 μ L from 1st tube to 2nd tube and mix. Transfer 300 μ L from 2nd tube to 3rd tube and mix, and so on.

Tube #	Volume to dilute	Volume of diluent	Concentration (ng/mL)
1	300 μ L of 100 ng/mL stock solution	300 μ L	50
2	300 μ L of tube #1	300 μ L	25
3	300 μ L of tube #2	300 μ L	12.5
4	300 μ L of tube #3	300 μ L	6.25
5	300 μ L of tube #4	300 μ L	3.125
6	300 μ L of tube #5	300 μ L	1.5625
7	300 μ L of tube #6	300 μ L	0.7813

Δ Note: The standard solutions are best used within 2 hours. The 100 ng/mL standard solution should be stored at 4°C for up to 12 hours, or at -20°C for up to 48 hours. Avoid repeated freeze-thaw cycles.

11. Sample Preparation

Store samples to be assayed within 24 hours at 4°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

- Serum: Allow the serum to clot in a serum separator tube (about 4 hours) at room temperature. Centrifuge at approximately 1,000 x g for 15 minutes. Analyze the serum immediately or aliquot and store samples at -20°C.
- Cell culture supernatant: Remove particulates by centrifugation, assay immediately or aliquot and store samples at -20°C.
- Plasma: Collect plasma using heparin or EDTA as an anticoagulant. Centrifuge for 15 minutes at 1,500 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at -20°C.
- Cell lysates: After sufficient splitting, there should be no obvious cell sediment. Centrifuge cell lysates at approximately 10,000 x g for 5 minutes. Collect the cell lysate supernatants. Assay immediately or aliquot and store samples at -20°C.

It is recommended to estimate the concentration of the target protein in the sample and select a proper dilution factor so that the diluted target protein concentration falls near the middle of the linear regime in the standard curve. Dilute the sample using the provided diluent buffer. The following is a guideline for sample dilution. Several trials may be necessary in practice. The sample must be well mixed with the diluents buffer.

- High target protein concentration (1,000 ng/mL-10,000 ng/mL). The working dilution is 1:100. i.e. Add 1 μ L sample into 99 μ L sample diluent buffer.
- Medium target protein concentration (100 ng/mL-1,000 ng/mL). The working dilution is 1:10. i.e. Add 10 μ L sample into 90 μ L sample diluent buffer.
- Low target protein concentration (1.56 ng/mL-100 ng/mL). The working dilution is 1:2. i.e. Add 50 μ L sample to 50 μ L sample diluent buffer.
- Very Low target protein concentration (0 ng/mL-1.56 ng/mL). No dilution necessary, or the working dilution is 1:2.

12. Assay Procedure

- It is recommended to assay all standards, controls and samples in duplicate.
 - The ABC working solution and TMB color developing agent must be kept warm at 37°C for 30 minutes before use. When diluting samples and reagents, they must be mixed completely and evenly. Standard LBP detection curve should be prepared for each experiment. The user will decide sample dilution fold by crude estimation of LBP amount in samples.
- 12.1** Aliquot 100 μ L per well of the 100 ng/mL, 50 ng/mL, 25 ng/mL, 12.5 ng/mL, 6.25 ng/mL, 3.125 ng/mL and 1.5625 ng/mL Human LBP standard solutions into the pre-coated 96-well plate.
 - 12.2** Add 100 μ L of the sample diluent buffer into the control well (Zero well).
 - 12.3** Add 100 μ L of each properly diluted sample of Human cell culture supernatants, cell lysates, tissue homogenates, serum or plasma (heparin, EDTA) to each empty well. See "Sample Preparation" above for details. It is recommended that each Human LBP standard solution and each sample be measured in duplicate.
 - 12.4** Seal the plate with a new adhesive cover provided and incubate at 37°C for 90 minutes.
 - 12.5** Remove the cover, discard plate content, and blot the plate onto paper towels or other absorbent material. Do NOT let the wells completely dry at any time.
 - 12.6** Add 100 μ L of biotinylated anti-Human LBP antibody working solution into each well, seal the plate with a new adhesive cover provided and incubate at 37°C for 60 minutes.
 - 12.7** Wash plate 3 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1 minute. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (Plate Washing Method: Discard the solution in the plate without touching the side walls. Blot the plate onto paper towels or other absorbent material. Soak each well with at least 300 μ L PBS or TBS buffer for 1~2 minutes. Repeat this process two additional times for a total of three washes. Note: For automated washing, aspirate all wells and wash three times with PBS or TBS buffer, overfilling wells with PBS

or TBS buffer. Blot the plate onto paper towels or other absorbent material.)

- 12.8** Add 100 μ L of prepared ABC working solution into each well, seal the plate with a new adhesive cover provided and incubate at 37°C for 30 minutes.
- 12.9** Wash plate 5 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1-2 minutes. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (See Step 12.7 for plate washing method.)
- 12.10** Add 90 μ L of prepared TMB color developing agent into each well, seal the plate with a new adhesive cover and incubate at 37°C in dark for 25-30 minutes.

Δ Note: For reference only, the optimal incubation time should be determined by end user. And the shades of blue can be seen in the wells with the four most concentrated Human LBP standard solutions; the other wells show no obvious color.

- 12.11** Add 100 μ L of prepared TMB Stop Solution into each well. The color changes into yellow immediately.
- 12.12** Read the O.D. absorbance at 450 nm in a microplate reader within 30 minutes after adding the TMB Stop Solution.

13. Calculations

The standard curve can be plotted as the relative O.D.450 of each standard solution (Y) vs. the respective concentration of the standard solution (X). The Human LBP concentration of the samples can be interpolated from the standard curve.

(the relative O.D.450) = (the O.D.450 of each well) – (the O.D.450 of Zero well).

Δ Note: if the samples measured were diluted, multiply the dilution factor to the concentrations from interpolation to obtain the concentration before dilution.

14. Typical data

Typical standard curve – Data provided for demonstration purposes only. A new standard curve must be generated for each assay performed.

Sample	Human LBP (ng/mL)	O.D.
1	0	0.103
2	1.56	0.217
3	3.12	0.289
4	6.25	0.463
5	12.5	0.731
6	25	1.175
7	50	1.903
8	100	2.402

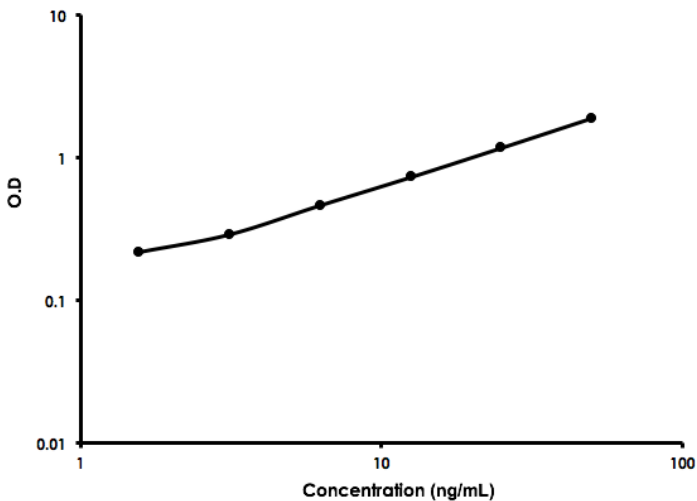


Figure 1. Human LBP ELISA Kit (ab213805) Standard Curve

15. Typical sample values

Sensitivity –

The biological sensitivity of the assay is <50 pg/mL.

The range is 0.78 ng/mL – 50 ng/mL.

Precision –

Intra-assay precision: (Precision within an assay) Three samples of known concentration were tested on one plate to assess intra-assay precision.

Sample	Number of measures	Mean (ng/mL)	Standard Deviation	CV%
1	16	15.3	0.66	4.3
2	16	38	1.9	5.0
3	16	85	4.76	5.6

Inter-assay precision: (Precision between assays) Three samples of known concentration were tested in separate assays to assess inter-assay precision.

Sample	Number of assays	Mean (ng/mL)	Standard Deviation	CV%
1	24	20	1.48	7.4
2	24	42	2.77	6.6
3	24	93	6.7	7.2

Specificity:

Natural and recombinant Human LBP.

Cross-reactivity:

There is no detectable cross-reactivity with other relevant proteins.

16. Troubleshooting

Problem	Cause	Solution
Poor standard curve	Inaccurate Pipetting	Check Pipettes
	Improper standard dilution	Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing
Low Signal	Incubation times too brief	Ensure sufficient incubation times standard/sample incubation
	Inadequate reagent volumes or improper dilution	Check Pipettes and ensure correct preparation
	Incubation times with TMB too brief	Ensure sufficient incubation time until blue color develops prior addition of TMB Stop Solution
Large CV	Plate is insufficiently washed	Review manual for proper wash technique. If using a plate washer, check all ports for obstructions.
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	All components 4°C. Keep TMB substrate solution protected from light.

17. Notes

Technical Support

Copyright © 2017 Abcam, All Rights Reserved. The Abcam logo is a registered trademark. All information / detail is correct at time of going to print.

Austria

wissenschaftlicherdienst@abcam.com | 019-288-259

France

supportscientifique@abcam.com | 01.46.94.62.96

Germany

wissenschaftlicherdienst@abcam.com | 030-896-779-154

Spain

soportecientifico@abcam.com | 91-114-65-60

Switzerland

technical@abcam.com

Deutsch: 043-501-64-24 | Français: 061-500-05-30

UK, EU and ROW

technical@abcam.com | +44(0)1223-696000

Canada

ca.technical@abcam.com | 877-749-8807

US and Latin America

us.technical@abcam.com | 888-772-2226

Asia Pacific

hk.technical@abcam.com | (852) 2603-6823

China

cn.technical@abcam.com | +86-21-5110-5938 | 400-628-6880

Japan

technical@abcam.co.jp | +81-(0)3-6231-0940

Singapore

sg.technical@abcam.com | 800 188-5244

Australia

au.technical@abcam.com | +61-(0)3-8652-1450

New Zealand

nz.technical@abcam.com | +64-(0)9-909-7829