

ab100768 – IL-1 Beta Rat ELISA Kit

Instructions for Use

For the quantitative measurement of rat IL-1 beta in cell lysates and tissue lysates.

This product is for research use only and is not intended for diagnostic use.

Table of Contents

INTRODUCTION

- 1. BACKGROUND 2
- 2. ASSAY SUMMARY 3

GENERAL INFORMATION

- 3. PRECAUTIONS 4
- 4. STORAGE AND STABILITY 4
- 5. MATERIALS SUPPLIED 4
- 6. MATERIALS REQUIRED, NOT SUPPLIED 5
- 7. LIMITATIONS 5
- 8. TECHNICAL HINTS 6

ASSAY PREPARATION

- 9. REAGENT PREPARATION 7
- 10. STANDARD PREPARATIONS 9
- 11. SAMPLE PREPARATION 11
- 12. PLATE PREPARATION 11

ASSAY PROCEDURE

- 13. ASSAY PROCEDURE 12

DATA ANALYSIS

- 14. CALCULATIONS 13
- 15. TYPICAL DATA 14
- 16. TYPICAL SAMPLE VALUES 15

RESOURCES

- 17. TROUBLESHOOTING 15
- 18. NOTES 17

1. BACKGROUND

Abcam's IL-1 beta Rat ELISA (Enzyme-Linked Immunosorbent Assay) Kit is an *in vitro* enzyme-linked immunosorbent assay for the quantitative measurement of rat IL-1 beta in cell lysates and tissue lysates.

This assay employs an antibody specific for rat IL-1 beta coated on a 96-well plate. Standards and samples are pipetted into the wells and IL-1 beta present in a sample is bound to the wells by the immobilized antibody. The wells are washed and biotinylated anti-rat IL-1 beta antibody is added. After washing away unbound biotinylated antibody, HRP-conjugated streptavidin is pipetted to the wells. The wells are again washed, a TMB substrate solution is added to the wells and colour develops in proportion to the amount of IL-1 beta bound. The Stop Solution changes the colour from blue to yellow, and the intensity of the colour is measured at 450 nm.

2. ASSAY SUMMARY

Primary Capture Antibody



Prepare all reagents, samples and standards as instructed.

Sample




Add standard or sample to each well used. Incubate at room temperature

Biotinylated Antibody



Add prepared biotin antibody to each well. Incubate at room temperature.

Streptavidin-HRP



Add prepared Streptavidin solution. Incubate at room temperature.

Substrate Colored Product



Add TMB One-Step Development Solution to each well. Incubate at room temperature. Add Stop Solution to each well. Read at 450nm immediately.

3. PRECAUTIONS

Please read these instructions carefully prior to beginning the assay.

Modifications to the kit components or procedures may result in loss of performance.

4. STORAGE AND STABILITY

Store kit at -20°C immediately upon receipt.

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in section 9. Reagent Preparation.

5. MATERIALS SUPPLIED

Item	Amount	Storage Condition (Before Preparation)
IL-1 beta Microplate (12 x 8 wells)	96 wells	-20°C
20X Wash Buffer Concentrate	25 mL	-20°C
Recombinant Rat IL-1 beta Standard	2 vials	-20°C
5X Sample Diluent Buffer	10 mL	-20°C
5X Assay Diluent	15 mL	-20°C
Biotinylated anti-rat IL-1 beta	2 vials	-20°C
200X HRP-Streptavidin Concentrate	200 µL	-20°C
TMB One-Step Substrate Reagent	12 mL	-20°C
Stop Solution	8 mL	-20°C
2X Cell Lysis Buffer	5 mL	-20°C

6. MATERIALS REQUIRED, NOT SUPPLIED

These materials are not included in the kit, but will be required to successfully utilize this assay:

- Microplate reader capable of measuring absorbance at 450 nm.
- Precision pipettes to deliver 2 μ L to 1 mL volumes.
- Adjustable 1-25 mL pipettes for reagent preparation.
- 100 mL and 1 liter graduated cylinders.
- Absorbent paper.
- Distilled or deionized water.
- Log-log graph paper or computer and software for ELISA data analysis.
- Tubes to prepare standard or sample dilutions.

7. LIMITATIONS

- Do not mix or substitute reagents or materials from other kit lots or vendors.

8. TECHNICAL HINTS

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers.
- Avoid foaming or bubbles when mixing or reconstituting components.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Ensure plates are properly sealed or covered during incubation steps.
- Complete removal of all solutions and buffers during wash steps.
- When preparing your standards, it is very critical to briefly spin down the vial first. The powder may drop off from the cap when opening it if you do not spin down. Be sure to dissolve the powder thoroughly when reconstituting. After adding Assay Diluent to the vial, we recommend inverting the tube a few times, then flick the tube a few times, and then spin it down; repeat this procedure 3-4 times. This is a technique we find very effective for thoroughly mixing the standard without too much mechanical force.
- Do not vortex the standard during reconstitution, as this will destabilize the protein.
- Once your standard has been reconstituted, it should be used right away or else frozen for later use.
- Keep the standard dilutions on ice while during preparation, but the ELISA procedure should be done at room temperature.
- Be sure to discard the working standard dilutions after use – they do not store well.
- **This kit is sold based on number of tests. A ‘test’ simply refers to a single assay well. The number of wells that contain sample, control or standard will vary by product. Review the protocol completely to confirm this kit meets your requirements. Please contact our Technical Support staff with any questions.**

9. REAGENT PREPARATION

Equilibrate all reagents to room temperature (18-25°C) prior to use.

9.1 1X Assay Diluent

5X Assay Diluent should be diluted 5-fold with deionized or distilled water before use.

9.2 1X Sample Diluent Buffer

5X Sample Diluent Buffer should be diluted 5-fold with deionized or distilled water before use.

9.3 1X Wash Solution

If the 20X Wash Concentrate contains visible crystals, equilibrate to room temperature and mix gently until dissolved. Dilute 20 mL of 20X Wash Buffer Concentrate into deionized or distilled water to yield 400 mL of 1X Wash Buffer.

9.4 1X Cell Lysate Buffer

2X Cell Lysate Buffer should be diluted 2-fold with deionized or distilled water (for cell lysate and tissue lysate).

9.5 1X Biotinylated IL-1 beta Detection Antibody

Briefly spin the Biotinylated anti-rat IL-1 beta vial before use. Add 100 µL of 1X Assay Diluent into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can either be stored at 4°C for 5 days or aliquoted and frozen at -20°C for 2 months). The detection antibody concentrate must be diluted 80-fold with 1X Assay Diluent prior to use in the Assay Procedure step 4.

9.6 **1X HRP-Streptavidin Solution**

Briefly spin the 200X HRP-Streptavidin concentrate vial and pipette up and down to mix gently before use. HRP-Streptavidin concentrate must be diluted 200-fold with 1X Assay Diluent prior to use in the Assay Procedure.

For example: Briefly spin the vial and pipette up and down to mix gently. Add 50 μ L of 200X HRP-Streptavidin concentrate into a tube with 10 mL 1X Assay Diluent to prepare a final 200 fold diluted 1X HRP-Streptavidin solution (don't store the diluted solution for next day use). Mix well.

10. STANDARD PREPARATIONS

- Prepare serially diluted standards immediately prior to use. Always prepare a fresh set of standards for every use.
- Standard (recombinant protein) should be stored at -20°C or -80°C (recommended at -80°C) after reconstitution.

10.1 Briefly spin the vial of IL-1 beta Standard. Prepare the 50,000 pg/mL **Stock Standard** by adding 400 μL 1X Sample Diluent Buffer into the vial (see table below).

10.2 Ensure the powder is thoroughly dissolved by gentle mixing.

10.3 Label tubes #1-7.

10.4 Pipette 260 μL 1X Sample Diluent Buffer into each tube.

10.5 Using the table below as a guide, prepare further serial dilutions.

10.6 1X Sample Diluent Buffer serves as the zero standard (0 pg/mL).

ASSAY PREPARATION

Standard Dilution Preparation Table

Standard #	Volume to Dilute (μL)	Diluent (μL)	Total Volume (μL)	Starting Conc. (pg/mL)	Final Conc. (pg/mL)
1	0	400	400	0	50,000
2	130	260	390	50,000	16,667
3	130	260	390	16,667	5,556
4	130	260	390	5,556	1,852
5	130	260	390	1,852	617.3
6	130	260	390	617.3	205.8
7	130	260	390	205.8	68.59
8	0	260	260	0	0



11. SAMPLE PREPARATION

General Sample Information:

- Tissue lysate and cell lysate sample should be diluted at least 5-fold with 1x Sample Diluent Buffer.
- Since different cells and tissues may contain different amounts of protein, as a starting point, we suggest using 500 μL of lysis buffer per 1×10^6 cells or 10 mg tissue. You may have to adjust this based upon your results. Your target total protein concentration of the homogenate should be at least 1,000 $\mu\text{g/mL}$, but 2,000 $\mu\text{g/mL}$ or more would be better.
- Centrifuge homogenized lysates to remove cell/tissue debris 5 min at 10,000 x g and save the supernatant. Lysates should be used or frozen as soon as possible and stored at -20°C or -80°C . Once frozen centrifuge them again before incubating with any immunoassay.

12. PLATE PREPARATION

- The 96 well plate strips included with this kit are supplied ready to use. It is not necessary to rinse the plate prior to adding reagents.
- Unused well strips should be returned to the plate packet and stored at 4°C .
- For statistical reasons, we recommend each sample should be assayed with a minimum of two replicates (duplicates).
- Well effects have not been observed with this assay. Contents of each well can be recorded on the template sheet included in the Resources section.

13. ASSAY PROCEDURE


- **Equilibrate all materials and prepared reagents to room temperature (18 - 25°C) prior to use.**
 - **It is recommended to assay all standards, controls and samples in duplicate.**
- 13.1. Add 100 μL of each standard and sample into appropriate wells. Cover well and incubate for 2.5 hours at room temperature or over night at 4°C with gentle shaking.
 - 13.2. Discard the solution and wash 4 times with 1X Wash Solution. Wash by filling each well with 1X Wash Solution (300 μL) using a multi-channel Pipette or auto washer. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
 - 13.3. Add 100 μL of 1X Biotinylated IL-1 beta Detection Antibody to each well. Incubate for 1 hour at room temperature with gentle shaking.
 - 13.4. Discard the solution. Repeat the wash as in step 13.2.
 - 13.5. Add 100 μL of 1X HRP-Streptavidin solution to each well. Incubate for 45 minutes at room temperature with gentle shaking.
 - 13.6. Discard the solution. Repeat the wash as in step 13.2.
 - 13.7. Add 100 μL of TMB One-Step Substrate Reagent to each well. Incubate for 30 minutes at room temperature in the dark with gentle shaking.
 - 13.8. Add 50 μL of Stop Solution to each well. Read at 450 nm immediately.

14. CALCULATIONS

Calculate the mean absorbance for each set of duplicate standards, controls and samples, and subtract the average zero standard optical density. Plot the standard curve on log-log graph paper, with standard concentration on the x-axis and absorbance on the y-axis. Draw the best-fit straight line through the standard points.

15. TYPICAL DATA

TYPICAL STANDARD CURVE – Data provided for **demonstration purposes only**. A new standard curve must be generated for each assay performed.

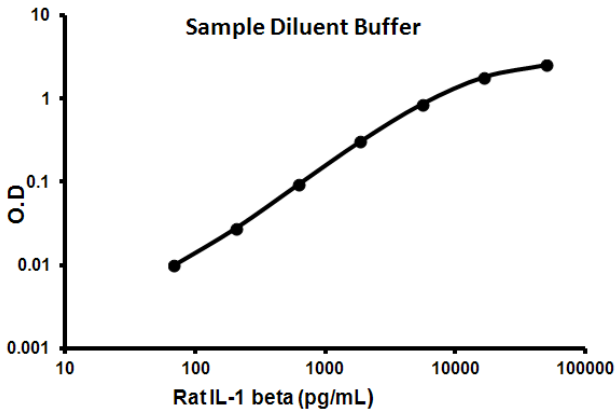

Conc. (pg/mL)	O.D.
	Sample Diluent Buffer
68.59	0.01
205.8	0.028
617.3	0.093
1852	0.305
5556	0.865
16,667	1.823
50,000	2.538

16. TYPICAL SAMPLE VALUES

SENSITIVITY –

The minimum detectable dose of IL-1 beta is typically less than 80 pg/mL.

RECOVERY –

Recovery was determined by spiking various levels of rat IL-1 beta into Rat tissue lysate and cell lysate. Mean recoveries are as follows:

Sample Type	Average % Recovery	Range (%)
Tissue lysate	136.5	126-145
Cell lysate	96.22	88-105

LINEARITY OF DILUTION -

Tissue Lysate	Average % Expected Value	Range (%)
1.2	110.8	99-118
1.4	135.4	125-142

Cell Lysate	Average % Expected Value	Range (%)
1.2	134.2	123-139
1.4	118.5	109-127

PRECISION –

	Intra-Assay	Inter-Assay
CV (%)	< 10%	< 12%

17. TROUBLESHOOTING

Problem	Cause	Solution
Poor standard curve	Inaccurate pipetting	Check pipettes
	Improper standards dilution	Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing
Low Signal	Incubation times too brief	Ensure sufficient incubation times; change to overnight standard/sample incubation
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
Large CV	Plate is insufficiently washed	Review manual for proper wash technique. If using a plate washer, check all ports for obstructions
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	Store the reconstituted protein at -80°C, all other assay components 4°C. Keep substrate solution protected from light.

18. NOTES

UK, EU and ROW

Email: technical@abcam.com | Tel: +44-(0)1223-696000

Austria

Email: wissenschaftlicherdienst@abcam.com | Tel: 019-288-259

France

Email: supportscientifique@abcam.com | Tel: 01-46-94-62-96

Germany

Email: wissenschaftlicherdienst@abcam.com | Tel: 030-896-779-154

Spain

Email: soportecientifico@abcam.com | Tel: 911-146-554

Switzerland

Email: technical@abcam.com

Tel (Deutsch): 0435-016-424 | Tel (Français): 0615-000-530

US and Latin America

Email: us.technical@abcam.com | Tel: 888-77-ABCAM (22226)

Canada

Email: ca.technical@abcam.com | Tel: 877-749-8807

China and Asia Pacific

Email: hk.technical@abcam.com | Tel: 400 921 0189 / +86 21 2070 0500

Japan

Email: technical@abcam.co.jp | Tel: +81-(0)3-6231-0940

www.abcam.com | www.abcam.cn | www.abcam.co.jp

Copyright © 2017 Abcam, All Rights Reserved. The Abcam logo is a registered trademark.

All information / detail is correct at time of going to print.