


CALCULATION OF RESULTS

Average the duplicate readings for each standard and sample, then subtract the average zero standard optical density (O.D.). Results may be normalized to total protein or cell number.

Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the human/mouse/rat SOD2 concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

TYPICAL DATA

A standard curve should be generated for each set of samples assayed. The graph below represents typical data generated when using the Human/Mouse/Rat Total SOD2/Mn-SOD DuoSet® IC ELISA. The standard curve was calculated using a computer generated 4-PL curve-fit. This standard curve is for demonstration purposes only.

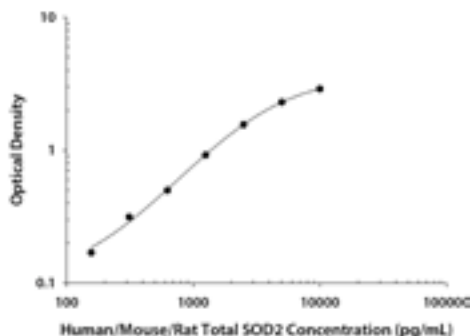

CALIBRATION

The Human/Mouse/Rat Total SOD2/Mn-SOD DuoSet® IC ELISA is calibrated against a highly purified *E. coli*-expressed recombinant human SOD2 produced at R&D Systems®. Samples containing natural SOD2 showed linear dilution parallel to the standard curve obtained using the Human/Mouse/Rat Total SOD2/Mn-SOD Standard. These results indicate that O.D. values from this DuoSet® IC ELISA can be used to determine the relative concentration of human/mouse/rat SOD2 in natural samples.

SPECIFICITY

The Human/Mouse/Rat Total SOD2/Mn-SOD DuoSet® IC ELISA specifically recognizes SOD2. Specificity was demonstrated by Western Blot analysis of the protein bound by the capture antibody supplied in the ELISA.

TECHNICAL HINTS & LIMITATIONS

- This DuoSet® IC ELISA should not be used beyond the expiration date on the kit label.
- Individual results may vary due to differences in technique, plasticware, and water sources.
- It is important that the diluents selected for reconstitution and for dilution of the samples and standard reflect the environment of the samples being measured. The diluents suggested in this protocol should be suitable for most cell lysates.
- The type of enzyme and substrate and the concentrations of capture/detection antibodies used can be varied to create an immunoassay with a different sensitivity and dynamic range. A basic understanding of immunoassay development is required for the successful use of these reagents in immunoassays.
- A thorough and consistent wash technique is essential for proper assay performance. Wash Buffer should be dispensed forcefully and removed completely from the wells by aspiration or decanting. Remove any remaining Wash Buffer by inverting the plate and blotting it against clean paper towels.
- Use a fresh reagent reservoir and pipette tips for each step.
- It is recommended that all standards and samples be assayed in duplicate.
- Avoid microbial contamination of reagents and buffers. This may interfere with the sensitivity of the assay. Buffers containing protein should be made under aseptic conditions and stored at 2-8 °C or be prepared fresh daily.

PRECAUTIONS

The Stop Solution recommended for use with this kit is an acid solution.

Some components in this kit contain a preservative which may cause an allergic skin reaction. Avoid breathing mist.

Color Reagent B recommended for use with this kit may cause skin, eye, and respiratory irritation. Avoid breathing fumes.

Wear protective gloves, clothing, eye, and face protection. Wash hands thoroughly after handling. Refer to the SDS on our website prior to use.

DuoSet® IC ELISA
INTRACELLULAR

Human/Mouse/Rat SOD2/Mn-SOD

Catalog Number: DYC3419-2 (2 plates)
DYC3419-5 (5 plates)

INTENDED USE

For the development of sandwich ELISAs to measure human, mouse, and rat Superoxide Dismutase-2/Manganese Superoxide Dismutase (SOD2/Mn-SOD) in cell lysates.

PRINCIPLE OF THE ASSAY

This DuoSet® IC ELISA contains the basic components required for the development of sandwich ELISAs to measure human/mouse/rat Superoxide Dismutase-2 (SOD2), also known as Manganese Superoxide Dismutase (Mn-SOD), in cell lysates. An immobilized capture antibody specifically binds human/mouse/rat SOD2. After washing away unbound material, a biotinylated detection antibody specific for human/mouse/rat SOD2 is used to detect the captured protein utilizing a standard Streptavidin-HRP format.

Note: The standard reconstitution method has changed. Read this package insert in its entirety before using this product.

This package insert must be read in its entirety before using this product.
For research use only. Not for use in diagnostic procedures.

Manufactured and Distributed by:

USA R&D Systems, Inc.
614 McKinley Place NE, Minneapolis, MN 55413
TEL: 800 343 7475 612 379 2956 FAX: 612 656 4400
E-MAIL: info@bio-techne.com

Distributed by:

Europe | Middle East | Africa Bio-Techne Ltd.
19 Barton Lane, Abingdon Science Park, Abingdon OX14 3NB, UK
TEL: +44 (0)1235 529449 FAX: +44 (0)1235 533420
E-MAIL: info.emea@bio-techne.com

China Bio-Techne China Co., Ltd.
Unit 1901, Tower 3, Raffles City Changning Office,
1193 Changning Road, Shanghai PRC 200051
TEL: +86 (21) 52380373 (400) 821-3475 FAX: +86 (21) 52371001
E-MAIL: info.cn@bio-techne.com

MATERIALS PROVIDED & STORAGE CONDITIONS

Store the unopened kit at 2-8 °C. Do not use past kit expiration date.

DESCRIPTION	PART #	CATALOG # DYC3419-2	CATALOG # DYC3419-5	STORAGE OF OPENED/ RECONSTITUTED MATERIAL
Human/Mouse/Rat Total SOD2/Mn-SOD Capture Antibody	842923	1 vial	2 vials	Store for up to 1 month at 2-8 °C or aliquot and store at ≤ -20 °C or ≤ -70 °C for up to 3 months in a manual defrost freezer.*
Human/Mouse/Rat Total SOD2/Mn-SOD Detection Antibody	842924	1 vial	2 vials	
Human/Mouse/Rat Total SOD2/Mn-SOD Standard	842925	3 vials	5 vials	Use within one hour of reconstitution. Use a fresh standard for each assay.
Streptavidin-HRP A	890803	1 vial	1 vial	Store for up to 3 months at 2-8 °C.* DO NOT FREEZE.

* Provided this is within the expiration date of the kit.

DYC3419-2 contains sufficient materials to run ELISAs on at least two 96 well plates.[†]
DYC3419-5 contains sufficient materials to run ELISAs on at least five 96 well plates.[†]

[†] Provided the following conditions are met:

- The reagents are prepared as described in this package insert.
- The assay is run as described in the General ELISA Protocol.
- The recommended microplates, buffers, diluents, substrates, and solutions are used.

OTHER MATERIALS REQUIRED

- Aprotinin (Tocris® # 4139).
- Leupeptin (Tocris® # 1167).
- Pepstatin (Tocris® # 1190).
- Phenylmethylsulfonyl Fluoride (PMSF) (Sigma # P7626).
- Sodium Orthovanadate (Na₃VO₄) (Sigma # S6508), activated.
- Sodium Pyrophosphate (Na₄P₂O₇) (Sigma # P8010).
- Sodium Fluoride (NaF) (Sigma # 201154).
- Sodium Azide (NaN₃) (Sigma # S2002).
- Triton™ X-100 (Sigma # T9284).
- Urea.
- Pipettes and pipette tips.
- Deionized or distilled water.
- 96 well microplates (R&D Systems®, Catalog # DY990).
- Plate sealers (R&D Systems®, Catalog # DY992).
- Squirt bottle, manifold dispenser, or automated microplate washer.

All trademarks and registered trademarks are the property of their respective owners.

SOLUTIONS REQUIRED

PBS - 137 mM NaCl, 2.7 mM KCl, 8.1 mM Na₂HPO₄, 1.5 mM KH₂PO₄, pH 7.2-7.4, 0.2 µm filtered (R&D Systems®, Catalog # DY006).

Wash Buffer - 0.05% Tween® 20 in PBS, pH 7.2-7.4 (R&D Systems®, Catalog # WA126).

Block Buffer - 1% BSA*, 0.05% NaN₃ in PBS, pH 7.2-7.4.

IC Diluent #1 - 1% BSA* in PBS, pH 7.2-7.4, 0.2 µm filtered.

IC Diluent #8** - 1 mM EDTA, 0.5% Triton X-100, 5 mM NaF in PBS, pH 7.2-7.4. **Note:** IC Diluent #8 is also the base diluent for IC Diluent #3, IC Diluent #7, and Lysis Buffer #6. Approximately 50 mL of this diluent is required to run the assay on one 96 plate.

IC Diluent #3** - 1 mM EDTA, 0.5% Triton X-100, 5 mM NaF, 1 M Urea in PBS, pH 7.2-7.4.

IC Diluent #7** - 1 mM EDTA, 0.5% Triton X-100, 5 mM NaF, 6 M Urea in PBS, pH 7.2-7.4.

Lysis Buffer #6** - 1 mM EDTA, 0.5% Triton X-100, 5 mM NaF, 6 M Urea, 1 mM activated Sodium Orthovanadate, 2.5 mM Sodium Pyrophosphate, 10 µg/mL Leupeptin, 10 µg/mL Pepstatin, 100 µM PMSF, 3.0 mg/mL Aprotinin in PBS, pH 7.2-7.4.

Substrate Solution - 1:1 mixture of Color Reagent A (H₂O₂) and Color Reagent B (Tetramethylbenzidine) (R&D Systems®, Catalog # DY999).

Stop Solution - 2 N H₂SO₄ (R&D Systems®, Catalog # DY994).

*The use of R&D Systems® Reagent Diluent Concentrate 2 (Catalog # DY995) or Millipore Bovine Serum Albumin, Fraction V, Protease free (Catalog # 82-045) is recommended. All buffers containing BSA must be stored at 2-8 °C.

**Alternatively, use Sample Diluent Concentrate 1 (5X) (R&D Systems®, Catalog # DYC001), prepared as described in the DYC001 insert.

REAGENT PREPARATION

Bring all reagents to room temperature before use.

Human/Mouse/Rat Total SOD2/Mn-SOD Capture Antibody (Part 842923) - Each vial contains 180 µg/mL of mouse anti-human SOD2 antibody when reconstituted with 200 µL of PBS.

Human/Mouse/Rat Total SOD2/Mn-SOD Detection Antibody (Part 842924) - Each vial contains 1.8 µg/mL of biotinylated goat anti-human SOD2 antibody when reconstituted with 1.0 mL of IC Diluent #1. Immediately before use, dilute the detection antibody to working concentration of 50 ng/mL using IC Diluent #1. Prepare only as much detection antibody as required to run each assay.

Human/Mouse/Rat Total SOD2/Mn-SOD Standard (Part 842925) **Reconstitute with a recommended volume of 500 µL of IC Diluent #7 to produce a stock solution. Refer to the vial label for the concentration of recombinant human SOD2.** Immediately before use, an initial 6-fold dilution should be made in IC Diluent #8. Additional dilutions should be made in IC Diluent #3. A seven point standard curve using 2-fold serial dilutions and a high standard of 20,000 pg/mL is recommended.

Streptavidin-HRP A (Part 890803) - 1.0 mL of Streptavidin conjugated to horseradish- peroxidase. Immediately before use, dilute the Streptavidin-HRP to the working concentration specified on the vial label using IC Diluent #1.

PREPARATION OF SAMPLES

Cell Lysates - Rinse cells two times with PBS, making sure to remove any remaining PBS after the second rinse. Solubilize cells at 1 x 10⁷ cells/mL in Lysis Buffer #6 and allow samples to sit on ice for 15 minutes. Assay immediately or store at ≤ -70 °C. Before use, centrifuge samples at 2000 x g for 5 minutes and transfer the supernate to a clean test tube. Sample protein concentration may be quantified using a total protein assay. For assaying, dilute lysates 6-fold with IC Diluent #8 and make further serial dilutions in IC Diluent #3.

Note: The final concentration of urea in all samples and standards should be 1 M prior to addition to the plate.

GENERAL ELISA PROTOCOL

Plate Preparation

1. Dilute the capture antibody to a working concentration of 1.0 µg/mL in PBS, without carrier protein. Immediately coat a 96 well microplate with 100 µL per well of the diluted capture antibody. Seal the plate and incubate overnight at room temperature.
2. Aspirate each well and wash with Wash Buffer, repeating the process two times for a total of 3 washes. Wash by filling each well with Wash Buffer (400 µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential for good performance. After the last wash, remove any remaining Wash Buffer by aspirating or by inverting the plate and blotting it against clean paper towels.
3. Block plates by adding 300 µL of Block Buffer to each well. Incubate at room temperature for 1-2 hours.
4. Repeat the aspiration/wash as in step 2. The plates are now ready for sample addition.

Assay Procedure

1. Add 100 µL of sample or standard in IC Diluent #3 per well. Use IC Diluent #3 as the zero standard. Cover with a plate sealer and incubate 2 hours at room temperature.
Note: A seven point standard curve using 2-fold serial dilutions and a high standard of 20,000 pg/mL is recommended.
2. Repeat the aspiration/wash as in step 2 of the Plate Preparation.
3. Add 100 µL of the diluted detection antibody to each well. Cover with a new plate sealer and incubate 2 hours at room temperature.
4. Repeat the aspiration/wash as in step 2 of the Plate Preparation.
5. Add 100 µL of the diluted Streptavidin-HRP A to each well. Incubate for 20 minutes at room temperature. Avoid placing the plate in direct light.
6. Repeat the aspiration/wash as in step 2 of Plate Preparation.
7. Add 100 µL of Substrate Solution to each well. Incubate for 20 minutes at room temperature. Avoid placing the plate in direct light.
8. Add 50 µL of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
9. Determine the optical density of each well immediately, using a microplate reader set to 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.