

ab157712 – C Reactive Protein (PTX1) Mouse ELISA Kit

Instructions for Use

For the quantitative measurement of C Reactive Protein (PTX1) in mouse serum, plasma and other biological samples.

This product is for research use only and is not intended for diagnostic use.

Table of Contents

INTRODUCTION

- 1. BACKGROUND 2
- 2. ASSAY SUMMARY 3

GENERAL INFORMATION

- 3. PRECAUTIONS 4
- 4. STORAGE AND STABILITY 4
- 5. MATERIALS SUPPLIED 4
- 6. MATERIALS REQUIRED, NOT SUPPLIED 5
- 7. LIMITATIONS 5
- 8. TECHNICAL HINTS 6

ASSAY PREPARATION

- 9. REAGENT PREPARATION 7
- 10. STANDARD PREPARATIONS 8
- 11. SAMPLE COLLECTION AND STORAGE 10
- 12. SAMPLE PREPARATION 11
- 13. PLATE PREPARATION 12

ASSAY PROCEDURE

- 14. ASSAY PROCEDURE 13

DATA ANALYSIS

- 15. CALCULATIONS 14
- 16. TYPICAL DATA 15
- 17. TYPICAL SAMPLE VALUES 16

RESOURCES

- 18. INTERFERENCES 17
- 19. TROUBLESHOOTING 17
- 20. NOTES 18

1. BACKGROUND

Abcam's C Reactive Protein (PTX1) Mouse ELISA kit is an *in vitro* enzyme-linked immunosorbent assay (ELISA) for the quantitative measurement of C Reactive Protein in Mouse samples.

In this assay the C Reactive Protein present in samples reacts with the anti-C Reactive Protein antibodies which have been adsorbed to the surface of polystyrene microtiter wells. After the removal of unbound proteins by washing, anti-C Reactive Protein antibodies conjugated with horseradish peroxidase (HRP) are added. These enzyme-labeled antibodies form complexes with the previously bound C Reactive Protein. Following another washing step, the amount of enzyme bound in complex is measured by the addition of a chromogenic substrate, 3,3',5,5'-tetramethylbenzidine (TMB). The quantity of bound enzyme varies proportionately with the concentration of C Reactive Protein in the sample tested; thus, the absorbance, at 450 nm, is a measure of the concentration of C Reactive Protein in the test sample. The quantity of C Reactive Protein in the test sample can be interpolated from the standard curve constructed from the standards, and corrected for sample dilution.

2. ASSAY SUMMARY

Primary capture antibody



Remove appropriate number of antibody coated well strips. Equilibrate all reagents to room temperature. Prepare all the reagents, samples, and standards as instructed.

Sample



Add standard or sample to each well used. Incubate at room temperature.

HRP conjugated antibody



Aspirate and wash each well. Add prepared HRP labeled secondary detector antibody. Incubate at room temperature

Substrate **Colored product**



Aspirate and wash each well. Add Chromogen Substrate Solution to each well. Immediately begin recording the color development

3. PRECAUTIONS

Please read these instructions carefully prior to beginning the assay.

All kit components have been formulated and quality control tested to function successfully as a kit. Modifications to the kit components or procedures may result in loss of performance.

4. STORAGE AND STABILITY

Store kit at +2-8°C immediately upon receipt.

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in section 9. Reagent Preparation.

5. MATERIALS SUPPLIED

Item	Amount	Storage Condition (Before Preparation)
Mouse C Reactive Protein ELISA Microplate	96 wells	2-8°C
Mouse C Reactive Protein Calibrator (lyophilized)	1 vial	2-8°C
5X Diluent Concentrate	50 mL	2-8°C
20X Wash Buffer Concentrate	50 mL	2-8°C
Enzyme-Antibody Conjugate	150 µL	2-8°C
Chromogen Substrate Solution	12 mL	2-8°C
Stop Solution	12 mL	2-8°C

6. MATERIALS REQUIRED, NOT SUPPLIED

These materials are not included in the kit, but will be required to successfully utilize this assay:

- Precision pipette (2 μ L to 200 μ L) for making and dispensing dilutions
- Test tubes
- Microtitre washer/aspirator
- Distilled or Deionized H₂O
- Microtitre Plate reader
- Assorted glassware for the preparation of reagents and buffer solutions
- Timer

7. LIMITATIONS

- Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of the information contained in the package insert instructions and with adherence to good laboratory practice
- Factors that might affect the performance of the assay include proper instrument function, cleanliness of glassware, quality of distilled or deionized water, and accuracy of reagent and sample pipettings, washing technique, incubation time or temperature
- Do not mix or substitute reagents with those from other lots or sources

8. TECHNICAL HINTS

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers
- Avoid foaming or bubbles when mixing or reconstituting components
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions
- Ensure plates are properly sealed or covered during incubation steps
- Complete removal of all solutions and buffers during wash steps

9. REAGENT PREPARATION

Equilibrate all reagents and samples to room temperature (18 - 25°C) prior to use.

9.1 1X Diluent Solution

The diluent solution is supplied as 5X Diluent Concentrate and must be diluted 1/5 with distilled or deionized water (1 part buffer concentrate, 4 parts dH₂O). The 1X Diluent Solution is stable for at least one week from the date of preparation and should be stored at 2 - 8°C.

9.2 1X Wash Buffer

The wash solution is supplied as 20X Concentrate and must be diluted 1/20 with distilled or deionized water (1 part buffer concentrate, 19 parts dH₂O). Crystal formation in the concentrate is not uncommon when storage temperatures are low. Warming of the concentrate to 30 - 35°C before dilution can dissolve crystals. The 1X Wash Buffer is stable for at least one week from the date of preparation and can be stored at room temperature (16 - 25°C) or at 2 - 8°C.

9.3 1X Enzyme-Antibody Conjugate

Calculate the required amount of 1X Enzyme-Antibody Conjugate solution for each microtitre plate test strip by adding 10 µL Enzyme-Antibody Conjugate to 990 µL of 1X Diluent for each test strip to be used for testing. Mix uniformly, but gently. Avoid foaming. The working conjugate solution is stable for up to 1 hour when stored in the dark.

9.4 Chromogen Substrate Solution

Ready to use as supplied.

9.5 Stop Solution

Ready to use as applied.

9.6 Mouse C Reactive Protein Calibrator

Add 1.0 mL of distilled or de-ionized water to the Mouse C Reactive Protein Calibrator and mix gently until dissolved. The amount of calibrator is shown on the vial, and after reconstitution

will have a concentration of $X \mu\text{g/mL}$, where X is the amount on the vial (the reconstituted calibrator should be aliquoted and stored frozen if future use is intended). Avoid multiple freeze-thaw cycles.

10. STANDARD PREPARATIONS

Prepare serially diluted standards immediately prior to use. Always prepare a fresh set of standards for every use.

10.1 Label tube numbers 1 - 6.

10.2 Prepare **Standard #1** by adding the appropriate volume of 1X Diluent Solution (see below) to tube #1. Add 60 μL of stock Mouse C Reactive Protein Calibrator to obtain a concentration at 25 ng/mL and mix thoroughly and gently.

*Example:

NOTE: This example is for demonstration purposes only. Please remember to check your calibrator vial for the actual concentration of calibrator provided.

C_S = Starting concentration of reconstituted Mouse C Reactive Protein Calibrator (variable e.g. 265.83 ng/mL)

C_F = Final concentration of Mouse C Reactive Protein Calibrator for the assay procedure (25 ng/mL)

V_A = Total volume of stock Mouse C Reactive Protein Calibrator to dilute (e.g. 60 μL)

V_D = Total volume of 1X Diluent Solution required to dilute stock Mouse C Reactive Protein Calibrator to prepare **Standard #1**

V_T = Total volume of **Standard #1**

D_F = Dilution factor

ASSAY PREPARATION

Calculate the dilution factor (D_F) between stock calibrator and the **Standard #1** final concentration:

$$C_S/C_F = D_F$$
$$265.83 / 25 = 10.63$$

Calculate the final volume V_D required to prepare the **Standard #1** at 25 ng/mL

$$V_A * D_F = V_T$$
$$V_D = V_T - V_A$$

$$60 * 10.63 = 638 \mu\text{L}$$
$$V_D = 638 - 60 = 578 \mu\text{L}$$

To tube #1, add 60 μL of reconstituted Mouse C Reactive Protein Calibrator to 578 μL of 1X Diluent Solution to obtain a concentration at 25 ng/mL (**Standard #1**).

- 10.3 Add 250 μL 1X Diluent Solution into tube numbers 2 - 6.
- 10.4 Prepare **Standard #2** by adding 250 μL Standard #1 to tube #2. Mix thoroughly and gently.
- 10.5 Prepare **Standard #3** by adding 250 μL from **Standard #2** to #3. Mix thoroughly and gently.
- 10.6 Using the table below as a guide to prepare further serial dilutions.
- 10.7 1X Diluent Solution serves as the zero standard (0 ng/mL).

ASSAY PREPARATION

Standard Dilution Preparation Table

Standard #	Volume to Dilute (μL)	Diluent (μL)	Total Volume (μL)	Starting Conc. (ng/mL)	Final Conc. (ng/mL)
1	See step 10.3				25
2	250	250	500	25	12.5
3	250	250	500	12.5	6.25
4	250	250	500	6.25	3.125
5	250	250	500	3.125	1.56
6	250	250	500	1.56	0.78



11. SAMPLE COLLECTION AND STORAGE

- 11.1 **Serum** – Blood should be collected by venipuncture. The serum should be separated from the cells after clot formation by centrifugation.
- 11.2 **Plasma** – For plasma samples, blood should be collected into a container with an anticoagulant and then centrifuged. Care should be taken to minimize hemolysis, excessive hemolysis can impact your results.

Assay immediately or aliquot and store samples at -20°C. Avoid repeated freeze-thaw cycles.

- **Precautions**

For any sample that might contain pathogens, care must be taken to prevent contact with open wounds.

- **Additives and Preservatives**

No additives or preservatives are necessary to maintain the integrity of the specimen. Avoid azide contamination.

12. SAMPLE PREPARATION

General Sample information:

The assay for quantification of C Reactive Protein in samples requires that each test sample be diluted before use. For a single step determination a dilution of 1/10 is appropriate for most serum/plasma samples. For absolute quantification, samples that yield results outside the range of the standard curve, a lesser or greater dilution might be required. If unsure of sample level, a serial dilution with one or two representative samples before running the entire plate is highly recommended.

- To prepare a 1/10 dilution of sample, transfer 25 μL of sample to 225 μL of 1X diluent. This gives you a 1/10 dilution. Mix thoroughly.

13. PLATE PREPARATION

- The 96 well plate strips included with this kit is supplied ready to use. It is not necessary to rinse the plate prior to adding reagents
- Unused well plate strips should be returned to the plate packet and stored at 4°C
- For each assay performed, a minimum of 2 wells must be used as blanks, omitting primary antibody from well additions
- For statistical reasons, we recommend each sample should be assayed with a minimum of two replicates (duplicates)
- Well effects have not been observed with this assay. Contents of each well can be recorded on the template sheet included in the Resources section

14. ASSAY PROCEDURE


- **Equilibrate all materials and prepared reagents to room temperature prior to use.**
- **It is recommended to assay all standards, controls and samples in duplicate.**
 - 14.1 Pipette 100 μ L of each standard, including zero control, in duplicate, into pre designated wells.
 - 14.2 Pipette 100 μ L of sample (in duplicate) into pre designated wells.
 - 14.3 Incubate the microtiter plate at room temperature for ten (10 ± 2) minutes. Keep plate covered and level during incubation.
 - 14.4 Following incubation, aspirate the contents of the wells.
 - 14.5 Completely fill each well with appropriately diluted 1X Wash Buffer and aspirate. Repeat three times, for a total of four washes. If washing manually: completely fill wells with wash buffer, invert the plate then pour/shake out the contents in a waste container. Follow this by gently striking the wells on absorbent paper to remove residual buffer. Repeat 3 times for a total of four washes.
 - 14.6 Pipette 100 μ L of appropriately 1X Enzyme-Antibody Conjugate to each well. Incubate at room temperature for ten (10 ± 2) minutes. Keep plate covered in the dark and level during incubation.
 - 14.7 Wash and blot the wells as described in 14.4 - 14.5.
 - 14.8 Pipette 100 μ L of TMB Substrate Solution into each well.
 - 14.9 Incubate in the dark at room temperature for precisely five (5) minutes.
 - 14.10 After five minutes, add 100 μ L of Stop Solution to each well.
 - 14.11 Determine the absorbance (450 nm) of the contents of each well. Calibrate the plate reader to manufacturer's specifications.

15. CALCULATIONS

Average the duplicate standard reading for each standard, sample and control blank. Subtract the control blank from all mean readings. Plot the mean standard readings against their concentrations and draw the best smooth curve through these points to construct a standard curve. Most plate reader software or graphing software can plot these values and curve fit. A four parameter algorithm (4PL) usually provides the best fit, though other equations can be examined to see which provides the most accurate (e.g. linear, semi-log, log/log, 4-parameter logistic). Extrapolate protein concentrations for unknown and control samples from the standard curve plotted. Samples producing signals greater than that of the highest standard should be further diluted in 1X Incubation Buffer and reanalyzed, then multiplying the concentration found by the appropriate dilution factor.

16. TYPICAL DATA

TYPICAL STANDARD CURVE – Data provided for **demonstration purposes only**. A new standard curve must be generated for each assay performed.

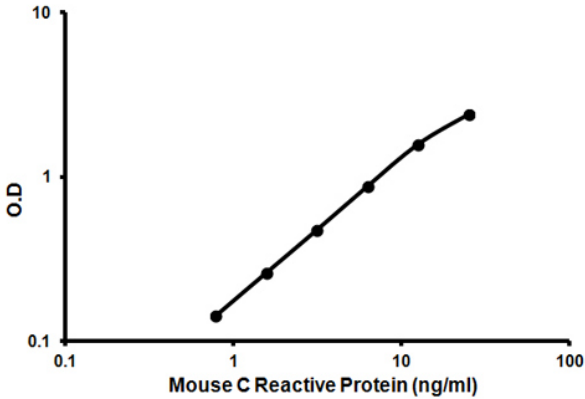

Standard Curve Measurements	
Conc. (ng/mL)	Mean O.D.
0.78	0.144
1.56	0.263
3.125	0.479
6.25	0.882
12.5	1.588
25	2.414

17. TYPICAL SAMPLE VALUES

SENSITIVITY –

Calculated minimum detectable dose = 0.1691 ng/mL

RECOVERY –

Control Serum Recovery = > 85%

PRECISION –

	% CV
Inter-Assay	< 10%
Intra-Assay	< 10%

18. INTERFERENCES

These chemicals or biologicals will cause interferences in this assay causing compromised results or complete failure.

Azide and thimerosal at concentrations higher than 0.1% inhibits the enzyme reaction.

19. TROUBLESHOOTING

Problem	Cause	Solution
Poor standard curve	Inaccurate pipetting	Check pipettes
	Improper standards dilution	Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing
Low Signal	Incubation times too brief	Ensure sufficient incubation times; change to overnight standard/sample incubation
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
Large CV	Plate is insufficiently washed	Review manual for proper wash technique. If using a plate washer, check all ports for obstructions
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	Store the reconstituted protein at -80°C, all other assay components 4°C. Keep substrate solution protected from light.

20. NOTES

UK, EU and ROW

Email: technical@abcam.com | Tel: +44-(0)1223-696000

Austria

Email: wissenschaftlicherdienst@abcam.com | Tel: 019-288-259

France

Email: supportscientifique@abcam.com | Tel: 01-46-94-62-96

Germany

Email: wissenschaftlicherdienst@abcam.com | Tel: 030-896-779-154

Spain

Email: soportecientifico@abcam.com | Tel: 911-146-554

Switzerland

Email: technical@abcam.com

Tel (Deutsch): 0435-016-424 | Tel (Français): 0615-000-530

US and Latin America

Email: us.technical@abcam.com | Tel: 888-77-ABCAM (22226)

Canada

Email: ca.technical@abcam.com | Tel: 877-749-8807

China and Asia Pacific

Email: hk.technical@abcam.com | Tel: 400 921 0189 / +86 21 2070 0500

Japan

Email: technical@abcam.co.jp | Tel: +81-(0)3-6231-0940

www.abcam.com | www.abcam.cn | www.abcam.co.jp