

# ab100704 – IL-1 beta Mouse ELISA Kit

## Instructions for Use

For the quantitative measurement of mouse IL-1 beta in plasma and cell culture supernatants.

- △ **Notes:** We have not been able to detect the endogenous Mouse IL-1 beta in normal serum with ab100704, only in serum spiked with Mouse IL-1 beta.

This product is for research use only and is not intended for diagnostic use.

# Table of Contents

---

## INTRODUCTION

1. BACKGROUND	2
2. ASSAY SUMMARY	3

## GENERAL INFORMATION

3. PRECAUTIONS	4
4. STORAGE AND STABILITY	4
5. MATERIALS SUPPLIED	4
6. MATERIALS REQUIRED, NOT SUPPLIED	5
7. LIMITATIONS	5
8. TECHNICAL HINTS	6

## ASSAY PREPARATION

9. REAGENT PREPARATION	7
10. STANDARD PREPARATIONS	8
11. SAMPLE PREPARATION	10
12. PLATE PREPARATION	10

## ASSAY PROCEDURE

13. ASSAY PROCEDURE	11
---------------------	----

## DATA ANALYSIS

14. CALCULATIONS	12
15. TYPICAL DATA	13
16. TYPICAL SAMPLE VALUES	15
17. ASSAY SPECIFICITY	16

## RESOURCES

18. TROUBLESHOOTING	17
19. NOTES	18

## 1. BACKGROUND

Abcam's IL-1 beta Mouse ELISA (Enzyme-Linked Immunosorbent Assay) kit is an *in vitro* enzyme-linked immunosorbent assay for the quantitative measurement of mouse IL-1 beta in plasma and cell culture supernatants. We have not been able to detect the endogenous Mouse IL-1 beta in normal serum with ab100704, only in serum spiked with Mouse IL-1 beta.

This assay employs an antibody specific for mouse IL-1 beta coated on a 96-well plate. Standards and samples are pipetted into the wells and IL-1 beta present in a sample is bound to the wells by the immobilized antibody. The wells are washed and biotinylated anti-mouse IL-1 beta antibody is added. After washing away unbound biotinylated antibody, HRP conjugated streptavidin is pipetted to the wells. The wells are again washed, a TMB substrate solution is added to the wells and color develops in proportion to the amount of IL-1 beta bound. The Stop Solution changes the color from blue to yellow, and the intensity of the color is measured at 450 nm.

## 2. ASSAY SUMMARY

### Primary Capture Antibody



Prepare all reagents, samples and standards as instructed.

### Sample




Add standard or sample to each well used. Incubate at room temperature

### Biotinylated Antibody



Add prepared biotin antibody to each well. Incubate at room temperature.

### Streptavidin-HRP



Add prepared Streptavidin solution. Incubate at room temperature.

### Substrate      Colored Product



Add TMB One-Step Development Solution to each well. Incubate at room temperature. Add Stop Solution to each well. Read at 450nm immediately.

### 3. PRECAUTIONS

**Please read these instructions carefully prior to beginning the assay.**

Modifications to the kit components or procedures may result in loss of performance.

### 4. STORAGE AND STABILITY

**Store kit at -20°C immediately upon receipt.**

Refer to list of materials supplied for storage conditions of individual components. Observe the storage conditions for individual prepared components in section 9. Reagent Preparation.

### 5. MATERIALS SUPPLIED

Item	Amount	Storage Condition (Before Preparation)
IL-1 beta Microplate (12 x 8 wells)	96 wells	-20°C
20X Wash Buffer Concentrate	25 mL	-20°C
Recombinant Mouse IL-1 beta Standard	2 vials	-20°C
Assay Diluent A	30 mL	-20°C
5X Assay Diluent B	15 mL	-20°C
Biotinylated anti-mouse IL-1 beta	2 vials	-20°C
200X HRP-Streptavidin Concentrate	200 µL	-20°C
TMB One-Step Substrate Reagent	12 mL	-20°C
Stop Solution	8 mL	-20°C

### **6. MATERIALS REQUIRED, NOT SUPPLIED**

These materials are not included in the kit, but will be required to successfully utilize this assay:

- Microplate reader capable of measuring absorbance at 450 nm.
- Precision pipettes to deliver 2  $\mu$ L to 1 mL volumes.
- Adjustable 1-25 mL pipettes for reagent preparation.
- 100 mL and 1 liter graduated cylinders.
- Absorbent paper.
- Distilled or deionized water.
- Log-log graph paper or computer and software for ELISA data analysis.
- Tubes to prepare standard or sample dilutions.

### **7. LIMITATIONS**

- Do not mix or substitute reagents or materials from other kit lots or vendors.

### 8. TECHNICAL HINTS

- Samples generating values higher than the highest standard should be further diluted in the appropriate sample dilution buffers.
- Avoid foaming or bubbles when mixing or reconstituting components.
- Avoid cross contamination of samples or reagents by changing tips between sample, standard and reagent additions.
- Ensure plates are properly sealed or covered during incubation steps.
- Complete removal of all solutions and buffers during wash steps.
- When preparing your standards, it is very critical to briefly spin down the vial first. The powder may drop off from the cap when opening it if you do not spin down. Be sure to dissolve the powder thoroughly when reconstituting. After adding Assay Diluent to the vial, we recommend inverting the tube a few times, then flick the tube a few times, and then spin it down; repeat this procedure 3-4 times. This is a technique we find very effective for thoroughly mixing the standard without too much mechanical force.
- Do not vortex the standard during reconstitution, as this will destabilize the protein.
- Once your standard has been reconstituted, it should be used right away or else frozen for later use.
- Keep the standard dilutions on ice while during preparation, but the ELISA procedure should be done at room temperature.
- Be sure to discard the working standard dilutions after use – they do not store well.
- **This kit is sold based on number of tests. A ‘test’ simply refers to a single assay well. The number of wells that contain sample, control or standard will vary by product. Review the protocol completely to confirm this kit meets your requirements. Please contact our Technical Support staff with any questions.**

## 9. REAGENT PREPARATION

Equilibrate all reagents to room temperature (18-25°C) prior to use.

### 9.1 1X Assay Diluent B

5X Assay Diluent B should be diluted 5-fold with deionized or distilled water before use.

### 9.2 1X Wash Solution

If the 20X Wash Concentrate contains visible crystals, equilibrate to room temperature and mix gently until dissolved. Dilute 20 mL of 20X Wash Buffer Concentrate into deionized or distilled water to yield 400 mL of 1X Wash Buffer.

### 9.3 1X Biotinylated IL-1 beta Detection Antibody

Briefly spin the Biotinylated anti-mouse IL-1 beta vial before use. Add 100  $\mu$ L of 1X Assay Diluent B into the vial to prepare a detection antibody concentrate. Pipette up and down to mix gently (the concentrate can either be stored at 4°C for 5 days or aliquoted and frozen at -20°C for 2 months). The detection antibody concentrate must be diluted 80-fold with 1X Assay Diluent B prior to use in the Assay Procedure.

### 9.4 1X HRP-Streptavidin Solution

Briefly spin the 200X HRP-Streptavidin concentrate vial and pipette up and down to mix gently before use. HRP-Streptavidin concentrate must be diluted 200-fold with 1X Assay Diluent B prior to use in the Assay Procedure.

For example: Briefly spin the vial and pipette up and down to mix gently. Add 75  $\mu$ L of 200X HRP-Streptavidin concentrate into a tube with 15 mL 1X Assay Diluent B to prepare a final 200 fold diluted 1X HRP-Streptavidin solution (don't store the diluted solution for next day use). Mix well.



## 10. STANDARD PREPARATIONS

- Prepare serially diluted standards immediately prior to use. Always prepare a fresh set of standards for every use.
- Standard (recombinant protein) should be stored at -20°C or -80°C (recommended at -80°C) after reconstitution.

10.1 Briefly spin the vial of IL-1 beta Standard. Prepare the 50 ng/mL **Stock Standard** by adding 400 µL Assay Diluent A (for plasma samples) or 1X Assay Diluent B (for cell culture culture medium) into the vial (see table below).

10.2 Ensure the powder is thoroughly dissolved by gentle mixing.

10.3 Label tubes #1-7.

10.4 Prepare **Standard #1** by adding 40 µL of the 50 ng/mL **Stock Standard**, to 960.0 µL of Assay Diluent A or 1X Assay Diluent B into tube 1#. Mix thoroughly and gently.

10.5 Pipette 400 µL of Assay Diluent A or 1X Assay Diluent B into remaining tubes.

10.6 Prepare **Standard #2** by adding 200 µL Standard #1 to tube #2 and mix thoroughly.

10.7 Prepare **Standard #3** by adding 200 µL Standard #2 to tube #3 and mix thoroughly.


10.8 Using the table below as a guide, prepare further serial dilutions.

10.9 Assay Diluent A or 1X Assay Diluent B serves as the zero standard (0 pg/mL).

# ASSAY PREPARATION

## Standard Dilution Preparation Table

Standard #	Volume to Dilute ( $\mu\text{L}$ )	Diluent ( $\mu\text{L}$ )	Total Volume ( $\mu\text{L}$ )	Starting Conc. ( $\text{pg/mL}$ )	Final Conc. ( $\text{pg/mL}$ )
1	40	960.0	1,000	50,000	2,000
2	200	400	600	2,000	666.7
3	200	400	600	666.7	222.2
4	200	400	600	222.2	74.07
5	200	400	600	74.07	24.69
6	200	400	600	24.69	8.23
7	200	400	600	8.23	2.74
8	0	400	400	0	0

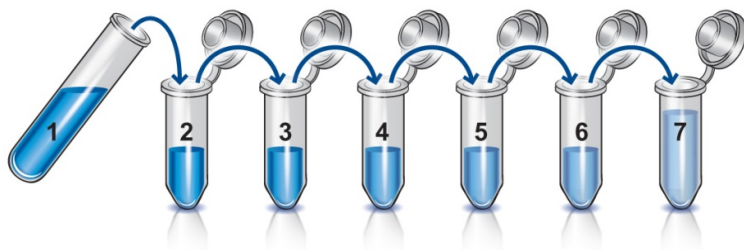

## 11. SAMPLE PREPARATION

### **General Sample Information:**

- Sample dilution: If your samples need to be diluted, Assay Diluent A should be used for dilution of plasma samples. 1X Assay Diluent B should be used for dilution of culture supernatants and urine.
- Suggested dilution for normal plasma: 2 fold.
- Please note that levels of the target protein may vary between different specimens. Optimal dilution factors for each sample must be determined by the investigator.

## 12. PLATE PREPARATION

- The 96 well plate strips included with this kit are supplied ready to use. It is not necessary to rinse the plate prior to adding reagents.
- Unused well strips should be returned to the plate packet and stored at 4°C.
- For statistical reasons, we recommend each sample should be assayed with a minimum of two replicates (duplicates).
- Well effects have not been observed with this assay. Contents of each well can be recorded on the template sheet included in the Resources section.

## **13. ASSAY PROCEDURE**



- **Equilibrate all materials and prepared reagents to room temperature (18 - 25°C) prior to use.**
  - **It is recommended to assay all standards, controls and samples in duplicate.**
- 13.1. Add 100  $\mu$ L of each standard (see Standard Preparation section 10) and sample into appropriate wells. Cover well and incubate for 2.5 hours at room temperature or over night at 4°C with gentle shaking.
  - 13.2. Discard the solution and wash 4 times with 1X Wash Solution. Wash by filling each well with 1X Wash Solution (300  $\mu$ L) using a multi-channel Pipette or auto washer. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
  - 13.3. Add 100  $\mu$ L of 1X Biotinylated IL-1 beta Detection Antibody (Reagent Preparation, section 9.3) to each well. Incubate for 1 hour at room temperature with gentle shaking.
  - 13.4. Discard the solution. Repeat the wash as in step 13.2.
  - 13.5. Add 100  $\mu$ L of 1X HRP-Streptavidin solution (see Reagent Preparation section 9.4) to each well. Incubate for 45 minutes at room temperature with gentle shaking.
  - 13.6. Discard the solution. Repeat the wash as in step 13.2.
  - 13.7. Add 100  $\mu$ L of TMB One-Step Substrate Reagent to each well. Incubate for 30 minutes at room temperature in the dark with gentle shaking.
  - 13.8. Add 50  $\mu$ L of Stop Solution to each well. Read at 450 nm immediately.

## **14. CALCULATIONS**

Calculate the mean absorbance for each set of duplicate standards, controls and samples, and subtract the average zero standard optical density. Plot the standard curve on log-log graph paper, with standard concentration on the x-axis and absorbance on the y-axis. Draw the best-fit straight line through the standard points.

## 15. TYPICAL DATA

**TYPICAL STANDARD CURVE** – Data provided for **demonstration purposes only**. A new standard curve must be generated for each assay performed.

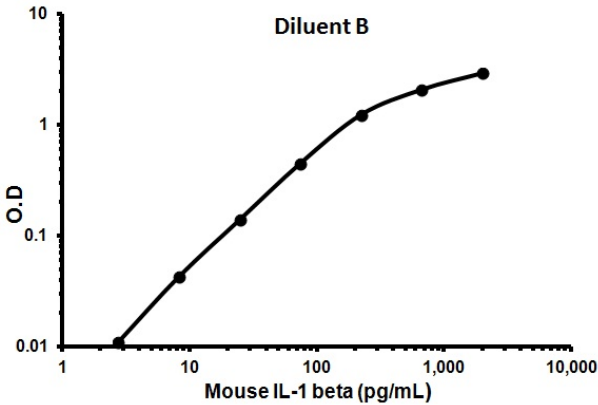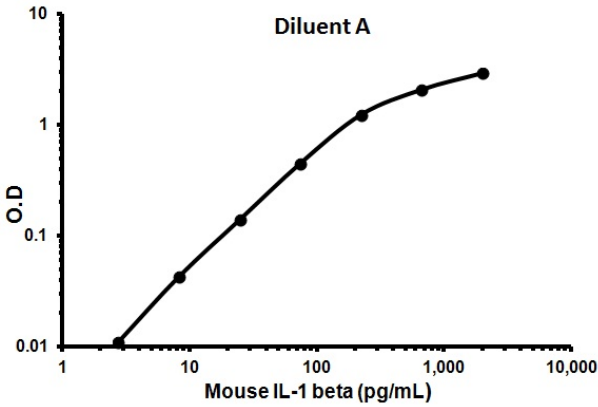

## DATA ANALYSIS

<b>Conc. (pg/mL)</b>	<b>O.D.</b>	
	<b>Assay Diluent A</b>	<b>Assay Diluent B</b>
2.74	0.011	0.011
8.23	0.043	0.043
24.69	0.140	0.140
74.07	0.452	0.452
222.22	1.240	1.240
666.67	2.087	2.087
2,000	2.934	2.934

## 16. TYPICAL SAMPLE VALUES

### SENSITIVITY –

The minimum detectable dose of IL-1 beta is typically less than 5 pg/mL.

### RECOVERY –

Recovery was determined by spiking various levels of mouse IL-1 beta into mouse plasma and cell culture media. Mean recoveries are as follows:

Sample Type	Average % Recovery	Range (%)
Plasma	99.24	90-109
Cell Culture Media	98.64	89-110

### LINEARITY OF DILUTION -

Plasma Dilution	Average % Expected Value	Range (%)
1:2	97	89-107
1:4	96	89-106

Cell Culture Media Dilution	Average % Expected Value	Range (%)
1:2	98	88-106
1:4	96	91-108

### PRECISION

	Intra-Assay	Inter-Assay
CV (%)	<10%	<12%



## **17. ASSAY SPECIFICITY**

Cross Reactivity: This ELISA kit shows no cross-reactivity with any of the cytokines tested (e.g., Mouse CD30, L CD30, T CD40, CRG-2, CTACK, CXCL16, Eotaxin, Eotaxin-2, Fas Ligand, Fractalkine, GCSF, GM-CSF, IFN- $\gamma$ , IGFBP-3, IGFBP-5, IGFBP-6, IL-1 $\alpha$ , IL-2, IL-3, IL-3 Rb, IL-4, IL-5, IL-6, IL-9, IL-10, IL-12 p40/p70, IL-12 p70, IL-13, IL-17, KC, Leptin R, LEPTIN(OB), LIX, L-Selectin, Lymphotactin, MCP-1, MCP-5, M-CSF, MIG, MIP-1 $\alpha$ , MIP-1 $\gamma$ , MIP-2, MIP-3 $\beta$ , MIP-3 $\alpha$ , PF-4, P-Selectin, RANTES, SCF, SDF-1 $\alpha$ , TARC, TCA-3, TECK, TIMP-1, TNF- $\alpha$ , TNFRI, TNFRII, TPO, VCAM-1, VEGF)..

## 18. TROUBLESHOOTING

<b>Problem</b>	<b>Cause</b>	<b>Solution</b>
Poor standard curve	Inaccurate pipetting	Check pipettes
	Improper standards dilution	Prior to opening, briefly spin the stock standard tube and dissolve the powder thoroughly by gentle mixing
Low Signal	Incubation times too brief	Ensure sufficient incubation times; change to overnight standard/sample incubation
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
Large CV	Inaccurate pipetting	Check pipettes
High background	Plate is insufficiently washed	Review manual for proper wash technique. If using a plate washer, check all ports for obstructions
	Contaminated wash buffer	Prepare fresh wash buffer
Low sensitivity	Improper storage of the ELISA kit	Store the reconstituted protein at -80°C, all other assay components 4°C. Keep substrate solution protected from light.

19. NOTES

**UK, EU and ROW**

Email: [technical@abcam.com](mailto:technical@abcam.com) | Tel: +44-(0)1223-696000

**Austria**

Email: [wissenschaftlicherdienst@abcam.com](mailto:wissenschaftlicherdienst@abcam.com) | Tel: 019-288-259

**France**

Email: [supportscientifique@abcam.com](mailto:supportscientifique@abcam.com) | Tel: 01-46-94-62-96

**Germany**

Email: [wissenschaftlicherdienst@abcam.com](mailto:wissenschaftlicherdienst@abcam.com) | Tel: 030-896-779-154

**Spain**

Email: [soportecientifico@abcam.com](mailto:soportecientifico@abcam.com) | Tel: 911-146-554

**Switzerland**

Email: [technical@abcam.com](mailto:technical@abcam.com)

Tel (Deutsch): 0435-016-424 | Tel (Français): 0615-000-530

**US and Latin America**

Email: [us.technical@abcam.com](mailto:us.technical@abcam.com) | Tel: 888-77-ABCAM (22226)

**Canada**

Email: [ca.technical@abcam.com](mailto:ca.technical@abcam.com) | Tel: 877-749-8807

**China and Asia Pacific**

Email: [hk.technical@abcam.com](mailto:hk.technical@abcam.com) | Tel: 400 921 0189 / +86 21 2070 0500

**Japan**

Email: [technical@abcam.co.jp](mailto:technical@abcam.co.jp) | Tel: +81-(0)3-6231-0940

[www.abcam.com](http://www.abcam.com) | [www.abcam.cn](http://www.abcam.cn) | [www.abcam.co.jp](http://www.abcam.co.jp)